



US008434242B2

(12) **United States Patent**  
**Hubbard et al.**

(10) **Patent No.:** **US 8,434,242 B2**  
(45) **Date of Patent:** **May 7, 2013**

- (54) **SPRAY DRIED HUMAN PLASMA**
- (71) Applicant: **Velico Medical, Inc.**, Beverly, MA (US)
- (72) Inventors: **Dennis Brian Hubbard**, Lancaster, MA (US); **Michael Haley**, Marlboro, MA (US)
- (73) Assignee: **Velico Medical, Inc.**, Beverly, MA (US)
- (\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

3,230,689	A	1/1966	Hussmann	
3,449,124	A	6/1969	Lipner	
3,507,278	A	4/1970	Werding	
3,644,128	A	2/1972	Lipner	
3,654,705	A	4/1972	Smith et al.	34/368
4,187,617	A	2/1980	Becker, Jr. et al.	
4,251,510	A	2/1981	Tankersley	
4,347,259	A	8/1982	Suzuki et al.	
4,358,901	A	11/1982	Takabatake et al.	
4,378,346	A	3/1983	Tankersley	
4,787,154	A	11/1988	Titus	34/92
5,096,537	A	3/1992	Bergquist et al.	

(Continued)

**FOREIGN PATENT DOCUMENTS**

CA	1182411	2/1985
CA	2065582	10/1992

(Continued)

- (21) Appl. No.: **13/680,283**
- (22) Filed: **Nov. 19, 2012**

- (65) **Prior Publication Data**  
US 2013/0078324 A1 Mar. 28, 2013

**Related U.S. Application Data**

- (63) Continuation of application No. 13/415,440, filed on Mar. 8, 2012, which is a continuation of application No. PCT/US2010/049176, filed on Sep. 16, 2010.

- (51) **Int. Cl.**  
**F26B 17/00** (2006.01)
- (52) **U.S. Cl.**  
USPC ..... **34/578**; 34/579; 34/580; 34/585;  
34/589; 239/406; 600/365
- (58) **Field of Classification Search** ..... 34/82, 83,  
34/201, 578, 579, 580, 585, 589; 239/404,  
239/406; 600/345, 36  
See application file for complete search history.

**References Cited**

**U.S. PATENT DOCUMENTS**

2,411,152	A	*	11/1946	Folsom	34/295
2,528,476	A	*	10/1950	Roos et al.	34/292
3,228,838	A	*	1/1966	Rinfret et al.	34/284

**OTHER PUBLICATIONS**

Civil Action Cover Sheet; *Entegriom, Inc. vs Velico Medical, Inc.*, dated Oct. 19, 2012.

(Continued)



*Primary Examiner* — Stephen M. Gravini

(74) *Attorney, Agent, or Firm* — Pierce Atwood LLP; Joseph M. Maraia

(57) **ABSTRACT**

The technology relates to spray dried plasma and methods of making the same. The method includes providing plasma to a spray drying apparatus, spray drying the plasma, at the spray drying apparatus, to form physiologically active plasma powder, the spray drying apparatus configured utilizing one or more parameters, and storing the physiologically active plasma powder.

**23 Claims, 33 Drawing Sheets**

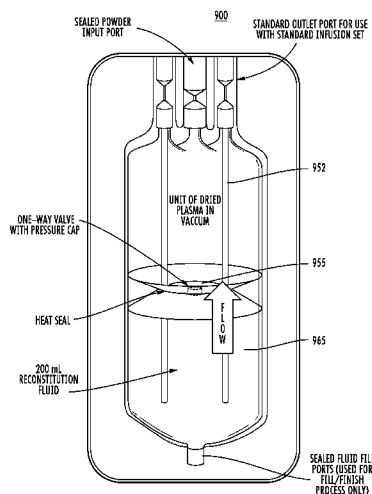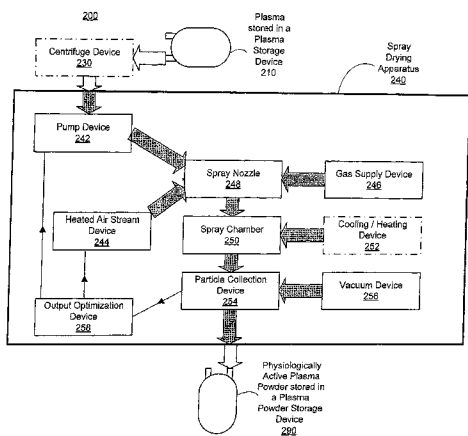

U.S. PATENT DOCUMENTS

5,145,706	A	9/1992	Hagi et al.	
5,252,221	A	10/1993	van Dommelen et al.	
5,372,811	A	12/1994	Yoder	
5,522,156	A *	6/1996	Ware	34/356
5,562,919	A	10/1996	Doty et al.	
5,575,999	A	11/1996	Yoder	
5,581,903	A	12/1996	Botich	
5,647,142	A	7/1997	Andersen et al.	
5,727,333	A *	3/1998	Folan	34/285
5,924,216	A	7/1999	Takahashi	
5,993,804	A	11/1999	Read et al.	
6,004,576	A	12/1999	Weaver et al.	
6,148,536	A *	11/2000	Iijima	34/92
6,308,434	B1 *	10/2001	Chickering et al.	34/373
6,345,452	B1 *	2/2002	Feuilloley et al.	34/437
6,463,675	B1	10/2002	Hansen et al.	
6,523,276	B1 *	2/2003	Meldrum	34/217
6,526,774	B1	3/2003	Lu et al.	
6,560,897	B2 *	5/2003	Chickering et al.	34/577
6,569,447	B2	5/2003	Kisic et al.	
6,582,654	B1 *	6/2003	Kral et al.	422/28
6,723,497	B2	4/2004	Wolkers et al.	
7,007,406	B2	3/2006	Wang et al.	
7,089,681	B2 *	8/2006	Herbert et al.	34/92
7,419,682	B2	9/2008	Campbell et al.	
7,527,805	B2	5/2009	Crenshaw et al.	
8,322,046	B2	12/2012	Wang et al.	
2002/0122803	A1	9/2002	Kisic et al.	
2002/0182195	A1	12/2002	Marguerre et al.	
2003/0037459	A1	2/2003	Chickering, III et al.	
2003/0099633	A1	5/2003	Campbell et al.	
2003/0103962	A1	6/2003	Campbell et al.	
2003/0143518	A1	7/2003	Luck et al.	
2003/0180283	A1	9/2003	Batycky et al.	
2003/0190314	A1	10/2003	Campbell et al.	
2004/0146565	A1	7/2004	Strohbehn et al.	
2004/0202660	A1	10/2004	Campbell et al.	
2005/0170068	A1	8/2005	Roodink et al.	
2005/0271674	A1	12/2005	Campbell et al.	
2006/0088642	A1	4/2006	Boersen et al.	
2006/0130768	A1	6/2006	Crenshaw et al.	
2006/0216687	A1	9/2006	Alves-Filho et al.	
2007/0014806	A1	1/2007	Marguerre et al.	
2008/0060213	A1 *	3/2008	Gehrmann et al.	34/284
2008/0138340	A1	6/2008	Campbell et al.	
2008/0145444	A1	6/2008	Merchant et al.	
2008/0213263	A1	9/2008	Campbell et al.	
2009/0092678	A1	4/2009	Marguerre et al.	
2009/0155410	A1	6/2009	Crenshaw et al.	
2010/0215667	A1	8/2010	Campbell et al.	
2012/0167405	A1 *	7/2012	Hubbard et al.	34/82

FOREIGN PATENT DOCUMENTS

CH	622683	4/1981
CN	1315139	10/2001
DE	3507278	9/1986
EP	0058903	9/1982
EP	1050220	11/2000
GB	573500	11/1945
GB	886533	1/1962
GB	964367	7/1964
GB	975786	11/1964
GB	1188168	4/1970
GB	2003042	3/1979
JP	56011903	2/1981

JP	63218201	9/1988
JP	01011618	1/1989
JP	03131302	6/1991
JP	03181301	8/1991
JP	5245301	9/1993
JP	5252910	10/1993
JP	10182124	A * 7/1998
JP	2002009037	A * 1/2002
JP	2005191275	A * 7/2005
JP	2007216158	A * 8/2007
WO	9615849	5/1996
WO	9618312	6/1996
WO	9738578	10/1997
WO	9907236	2/1999
WO	9907390	2/1999
WO	0056166	9/2000
WO	0172141	10/2001
WO	02078741	10/2002
WO	02078742	10/2002
WO	02/092213	11/2002
WO	03030654	4/2003
WO	03030918	4/2003
WO	03063607	8/2003
WO	2004075988	9/2004
WO	2007036227	4/2007
WO	2008/122288	10/2008
WO	2010117976	10/2010

OTHER PUBLICATIONS

Complaint including Exhibit A, B, and C; *Entegriion, Inc. vs Velico Medical, Inc.*, dated Oct. 19, 2012.

Mini Spray Dryer B-290—Application Note; [www.buchi.com](http://www.buchi.com); Mar. 30, 2008.

Nano Spray Dryer B-90; [www.buchi.com](http://www.buchi.com); Jul. 18, 2011.

Mini Spray Dryer System Configuration; [www.buchi.com](http://www.buchi.com); Jan. 8, 2007.

Quick Operation Guide; Mini Spray Dryer B-290; [www.buchi.com](http://www.buchi.com); Sep. 16, 2004.

Process Parameters; [www.buchi.com](http://www.buchi.com); Nov. 21, 2008.

Training Papers Spray Drying; Version B; [www.buchi.com](http://www.buchi.com); 19 pages; Oct. 29, 2002.

Mini Spray Dryer B-290; [www.buchi.com](http://www.buchi.com); May 10, 2007.

Operation Manual; Mini Spray Dryer B-290; Version G; [www.buchi.com](http://www.buchi.com); mailed Feb. 8, 2007.

PCT International Search Report and Written Opinion; PCT/US2010/049176; Sep. 16, 2010.

Edwards et al., The Preparation and Use of Dried Plasma for Transfusion; *British Medical journal*; vol. 1, No. 4131; Mar. 9, 1940; pp. 377-381.

PCT International Search Report from International Application No. PCT/US2011/058358, filed Oct. 28, 2011, mailed Jul. 4, 2012.

Answer, Affirmative Defenses, Counterclaims, Cross-Claims and Jury Demand, *Entegriion, Inc. vs Velico Medical, Inc.*, Dated: Dec. 3, 2012.

Entegriion'S Reply to Counterclaims; *Entegriion, Inc. vs Velico Medical, Inc.*; Dated: Jan. 14, 2013.

Entegriion'S Motion to Dismiss Counts I, II, V, VI and XI of Velico Medical, Inc's Counterclaims and Memorandum in Support of Entegriion'S Motion to Dismiss Counts I, II, V, VI, and XI of Velico Medical, Inc.'s Counterclaims; *Entegriion, Inc. vs Velico Medical, Inc.*; Dated: Jan. 14, 2013.

\* cited by examiner

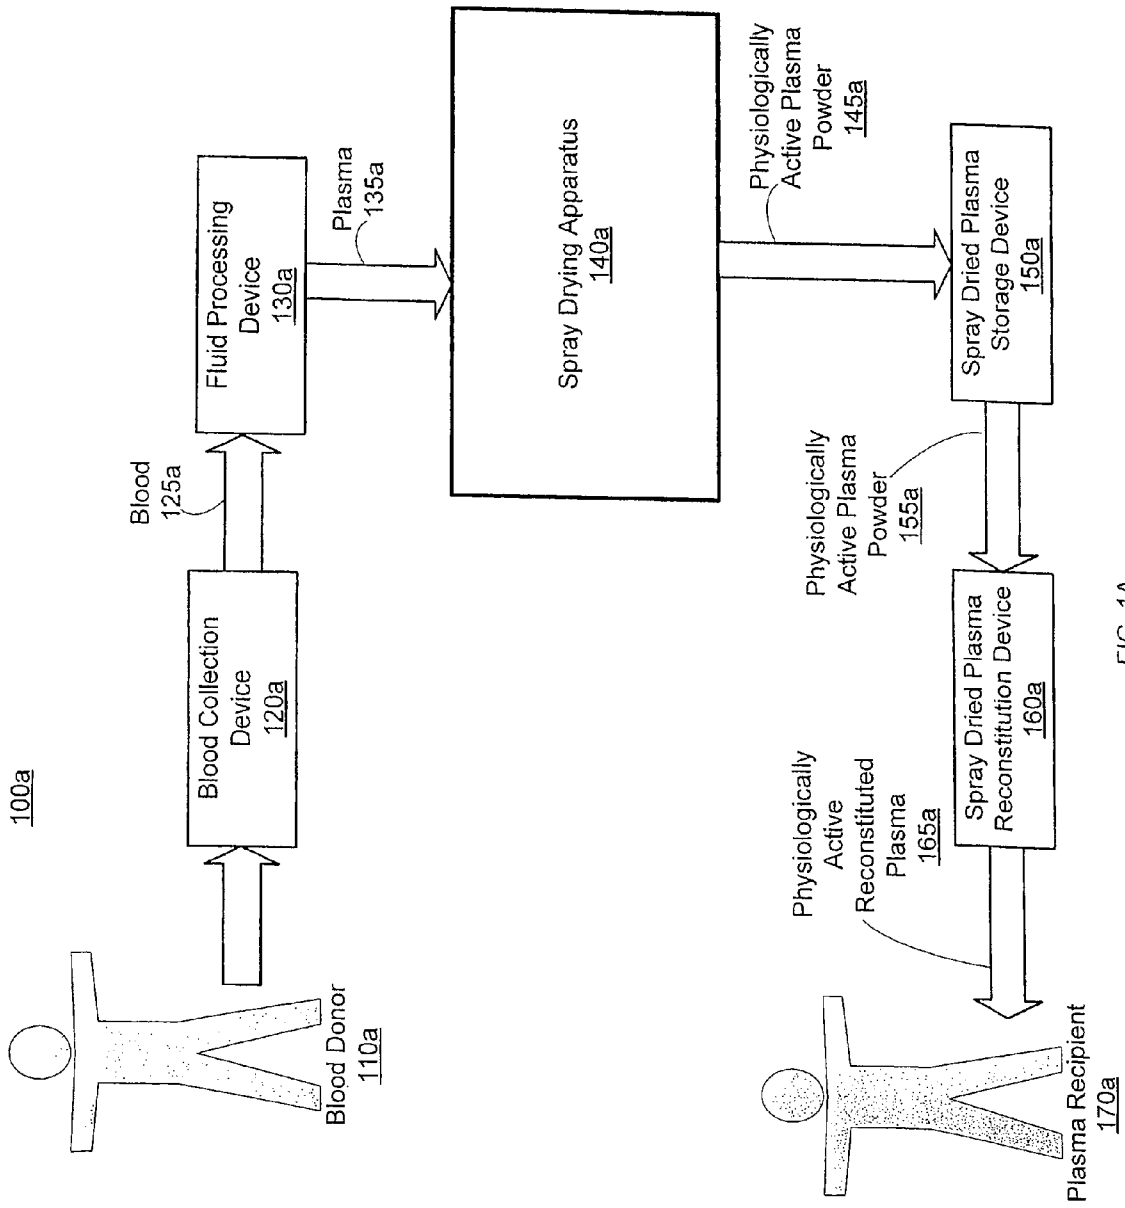


FIG. 1A

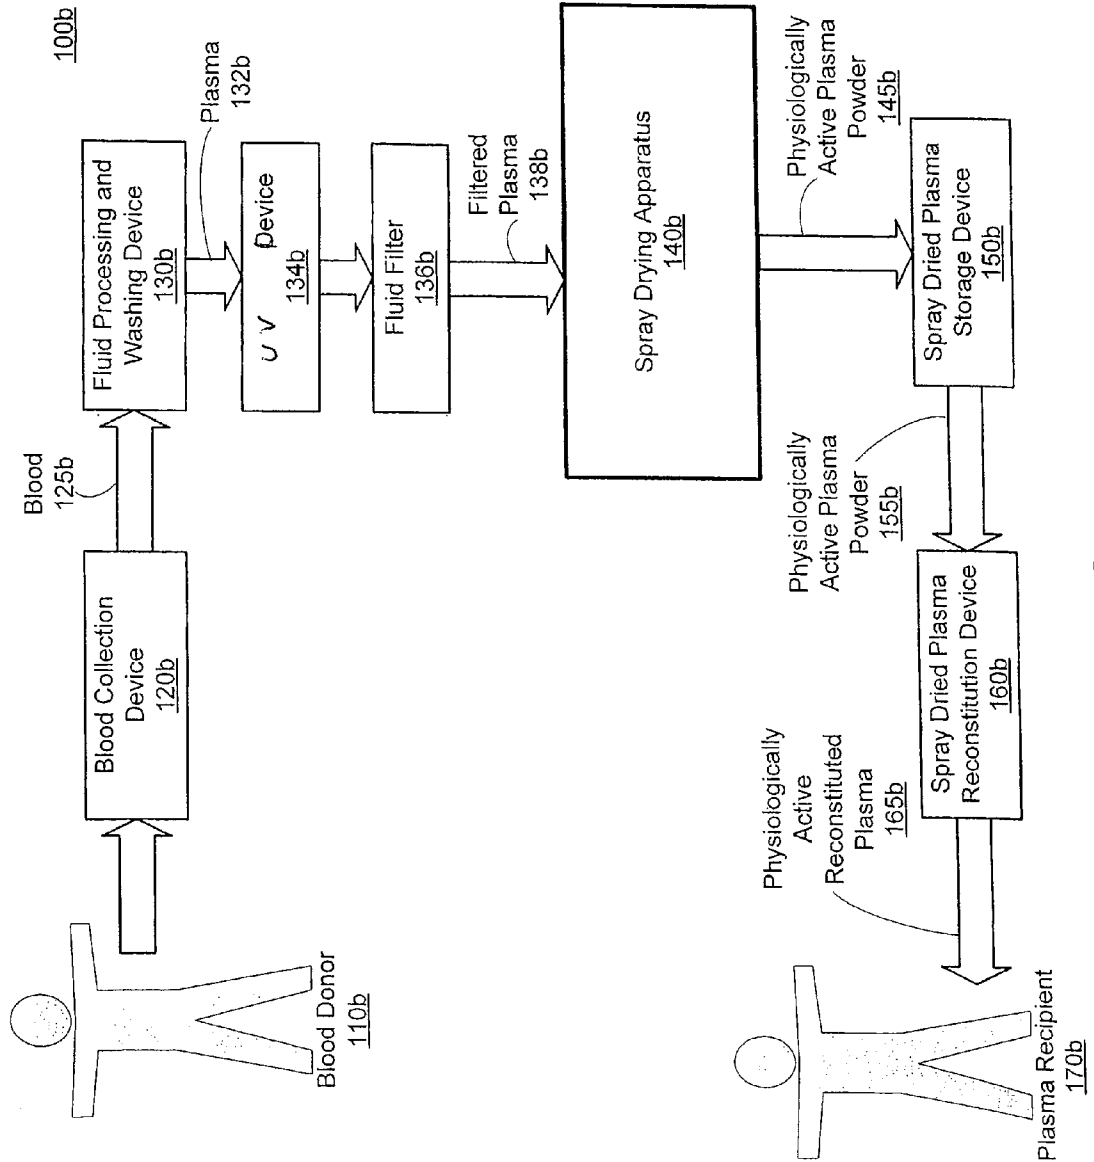


FIG. 1B

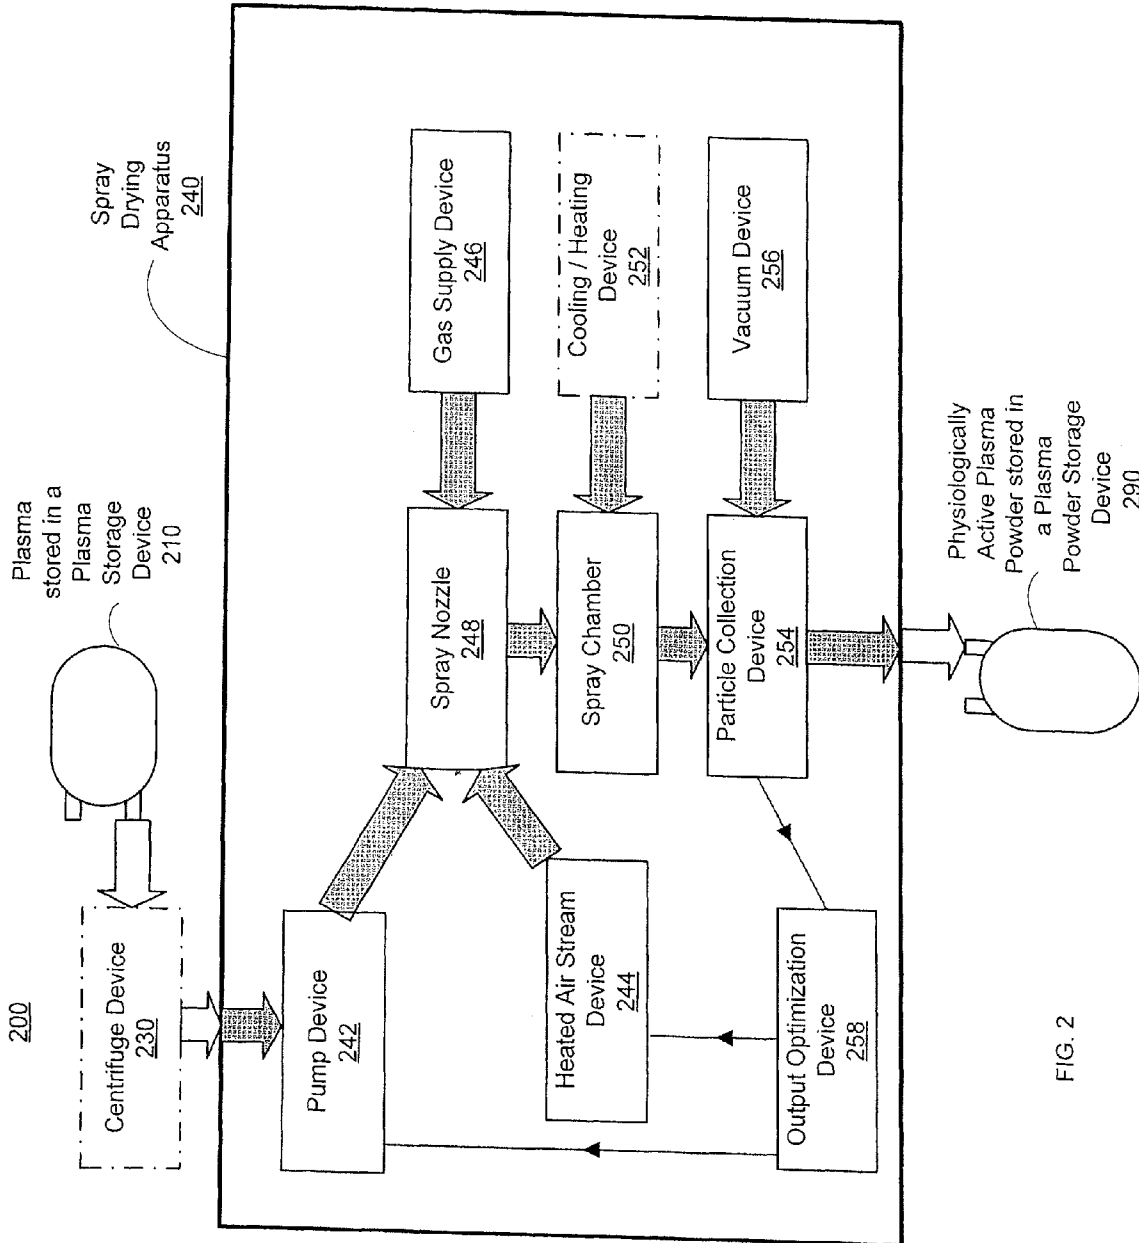


FIG. 2

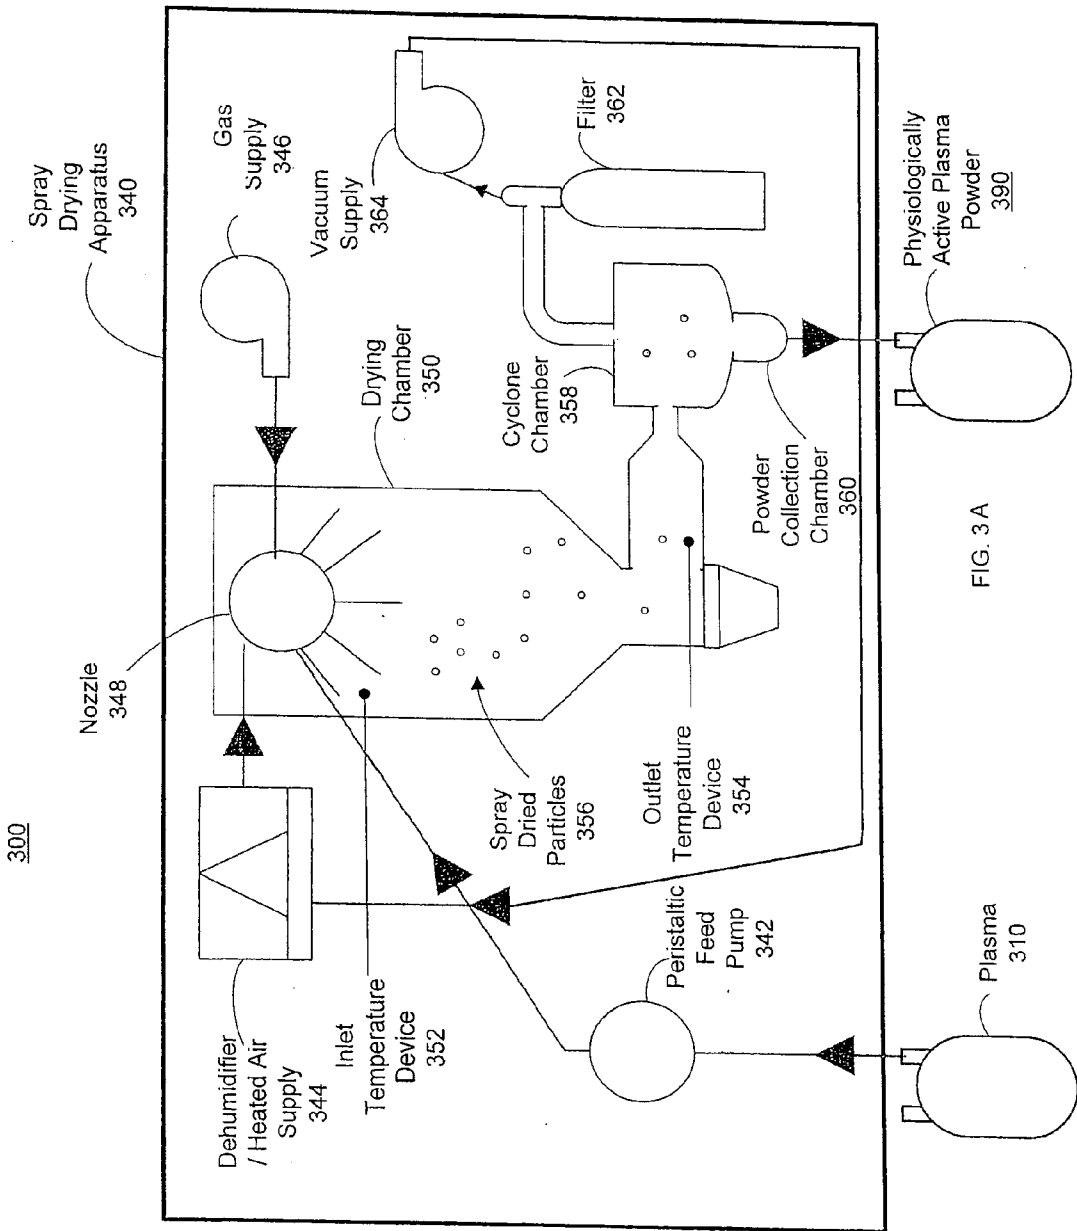
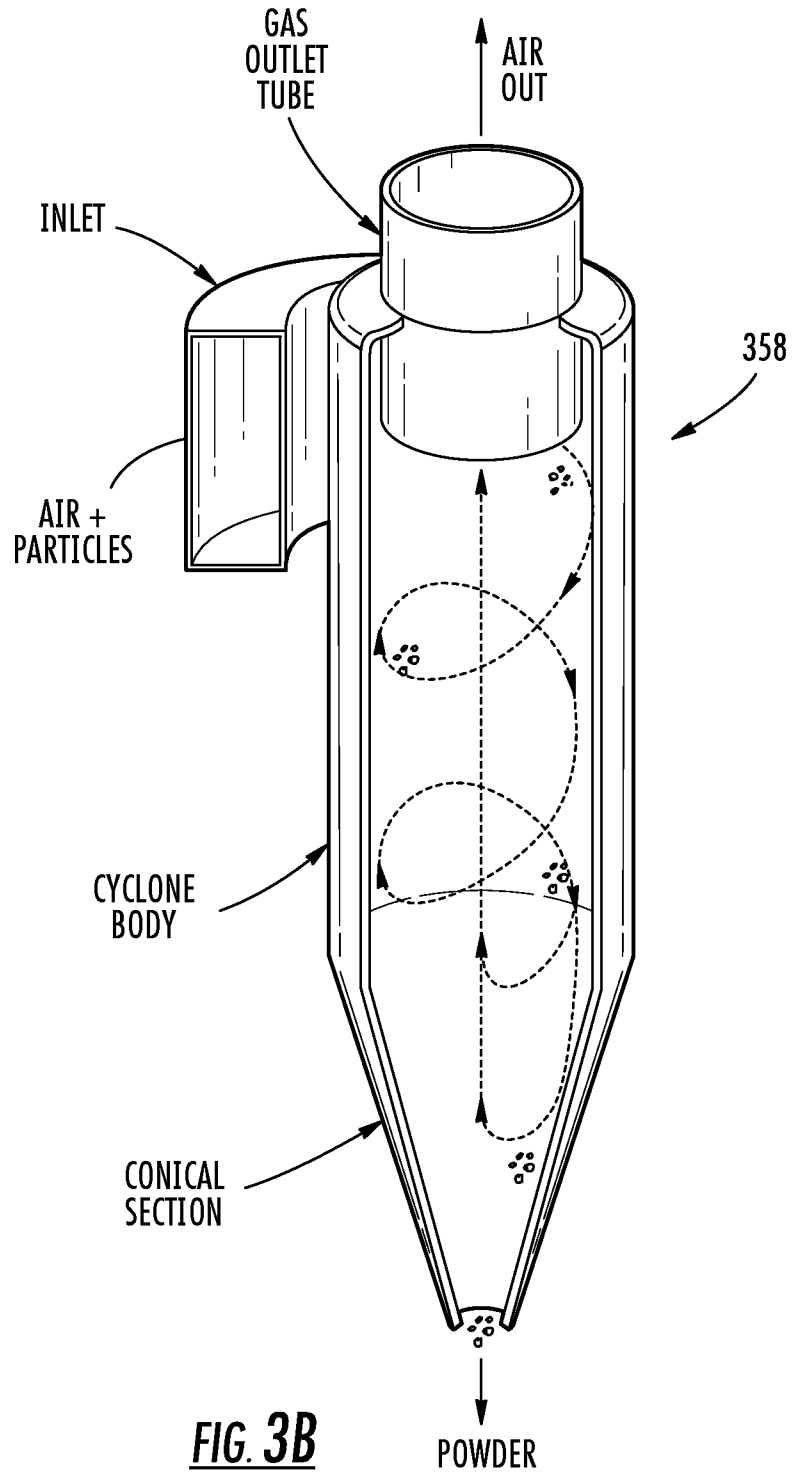


FIG. 3A



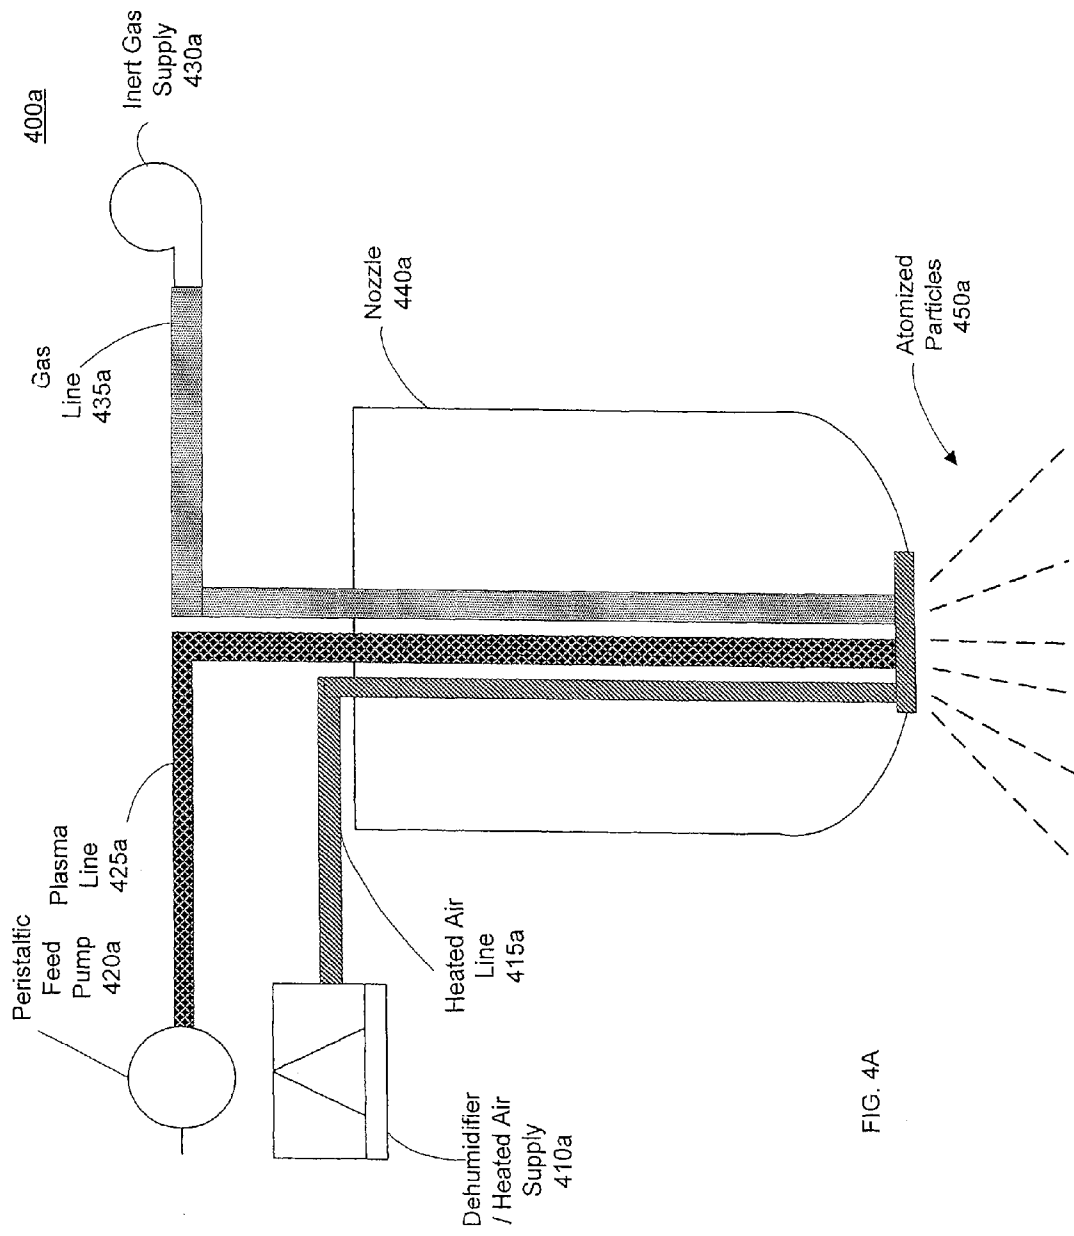


FIG. 4A



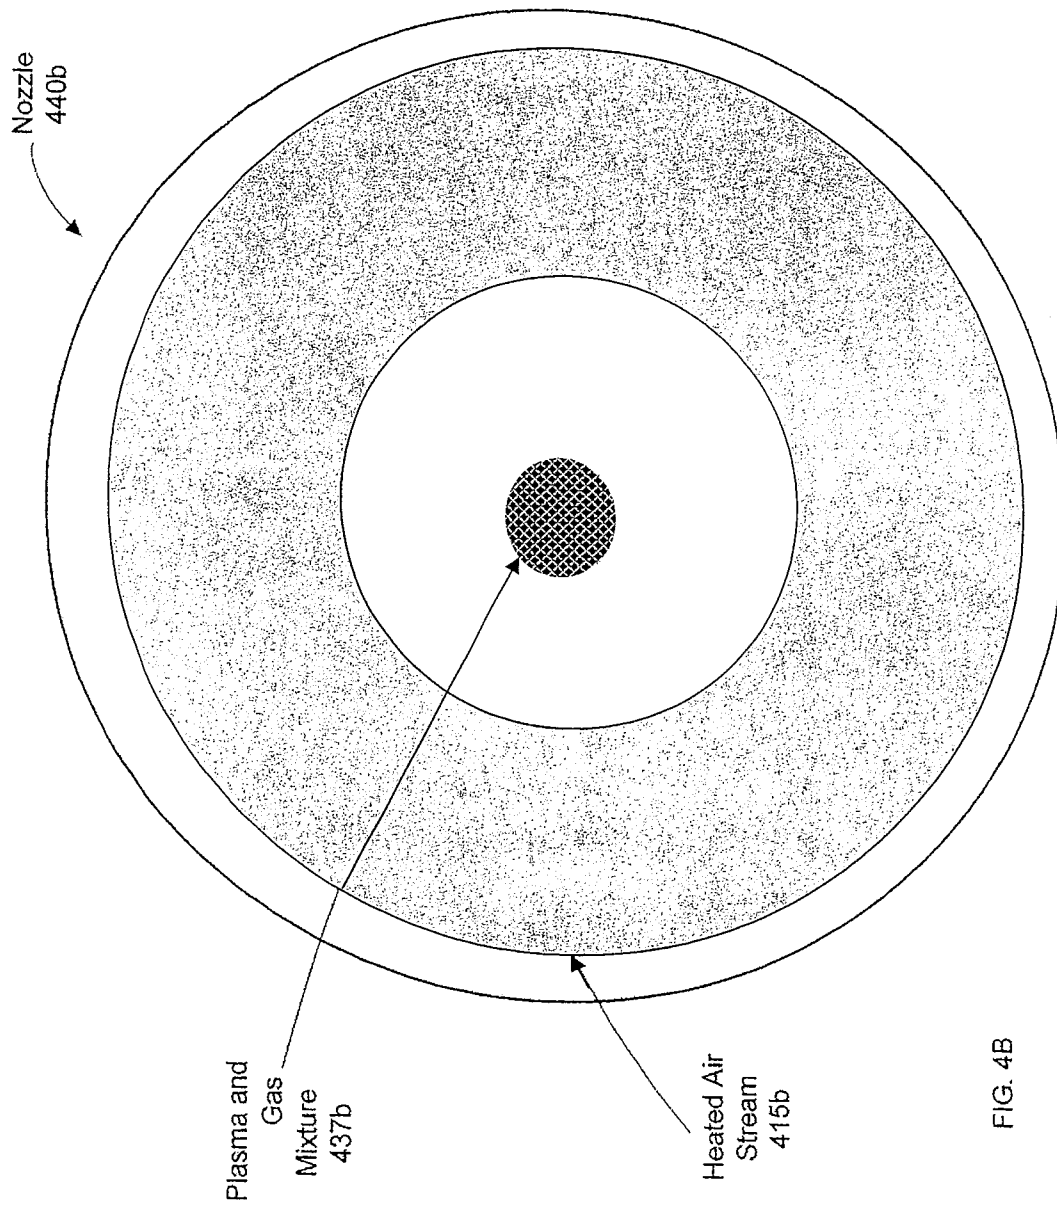


FIG. 4B

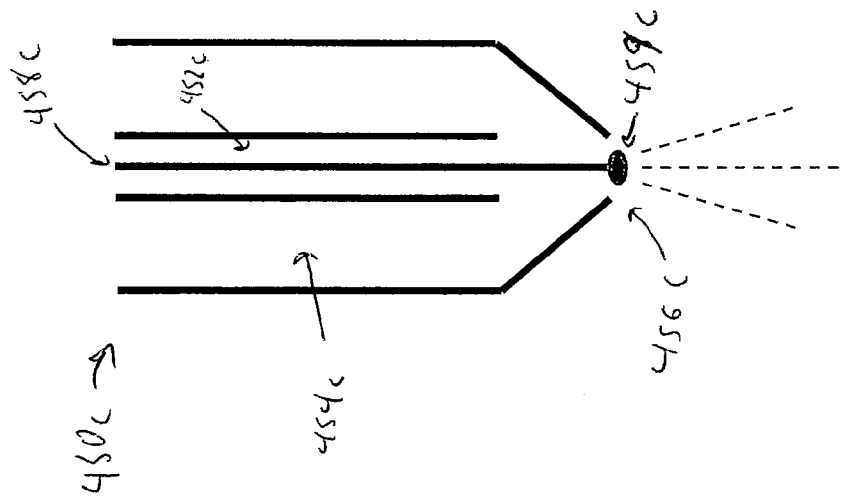


Fig. 4C

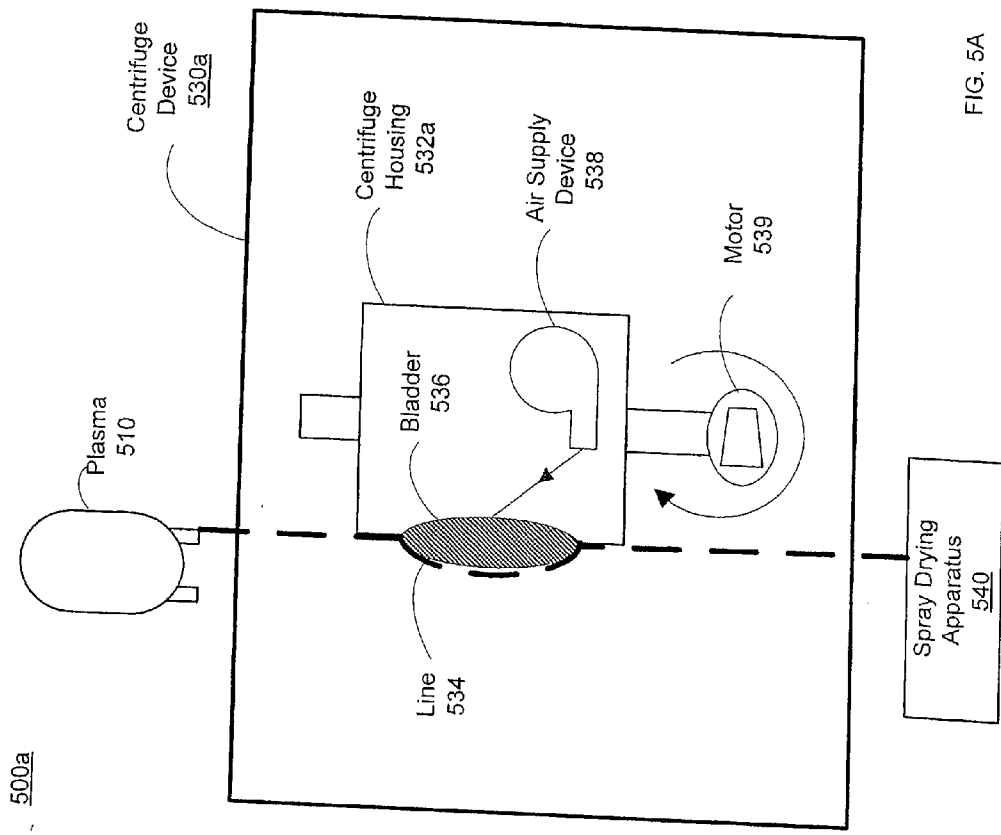


FIG. 5A

500a

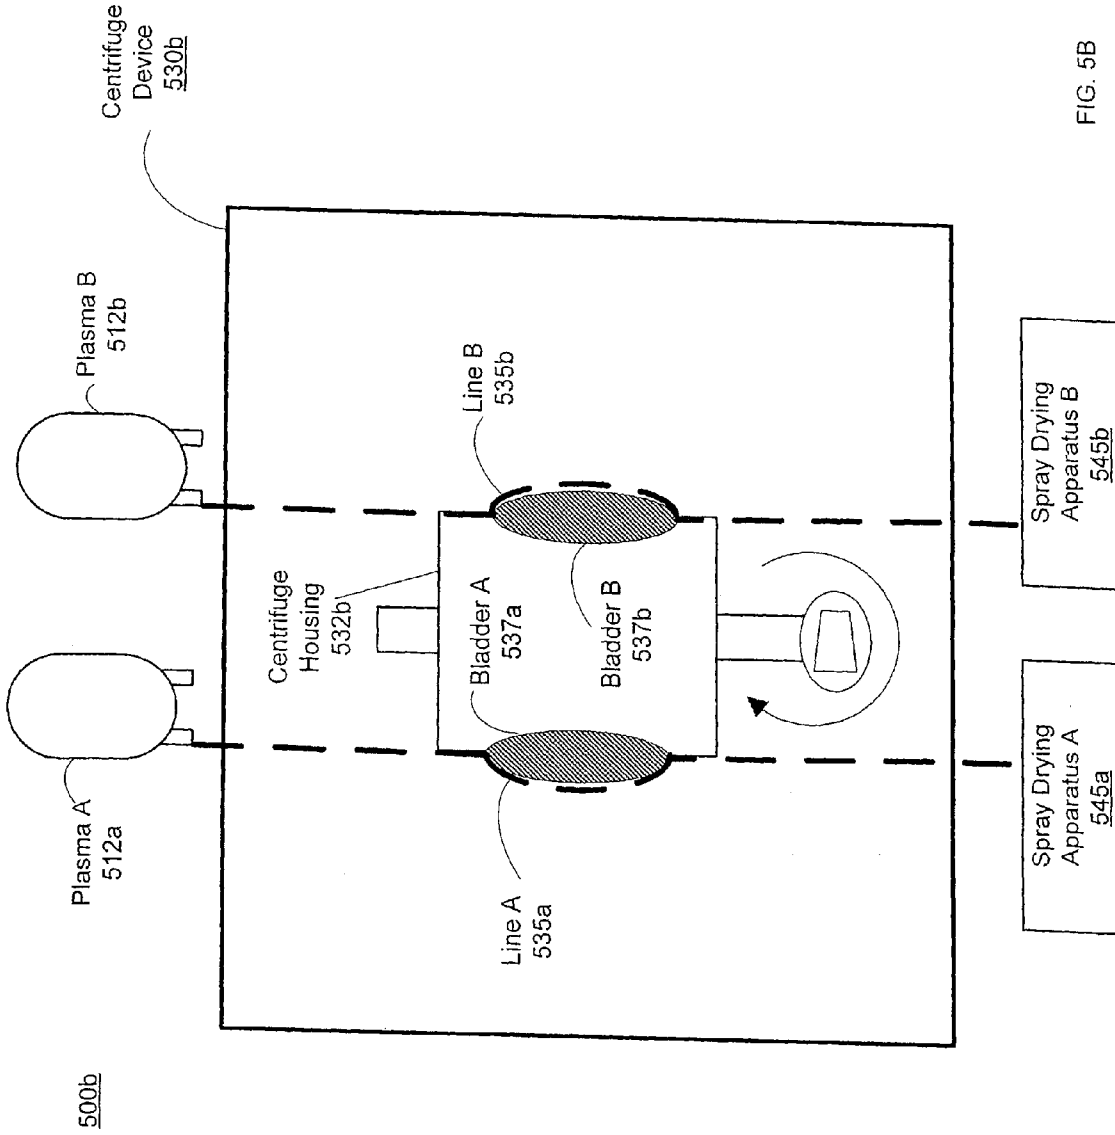


FIG. 5B

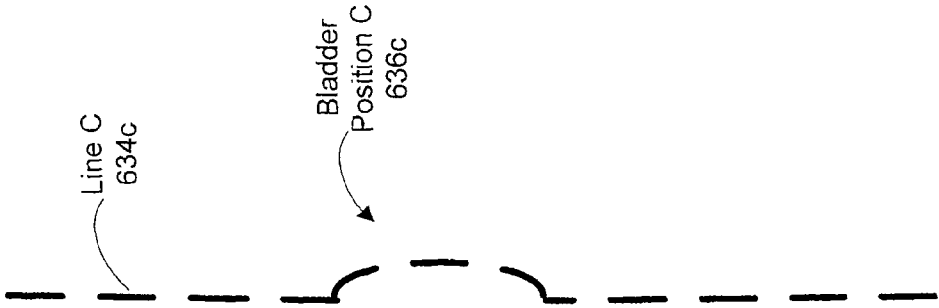


FIG. 6A

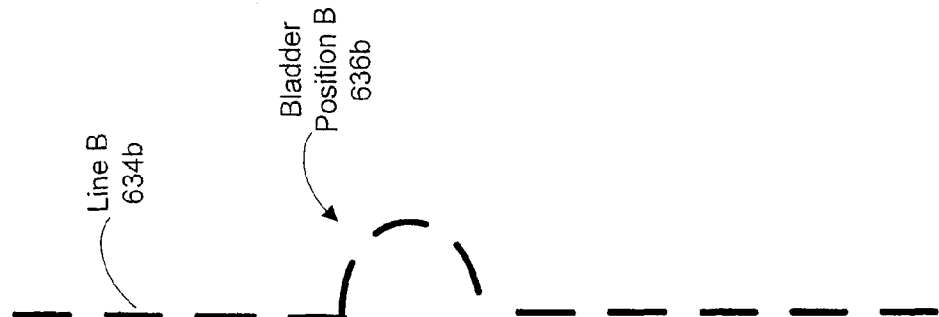


FIG. 6B

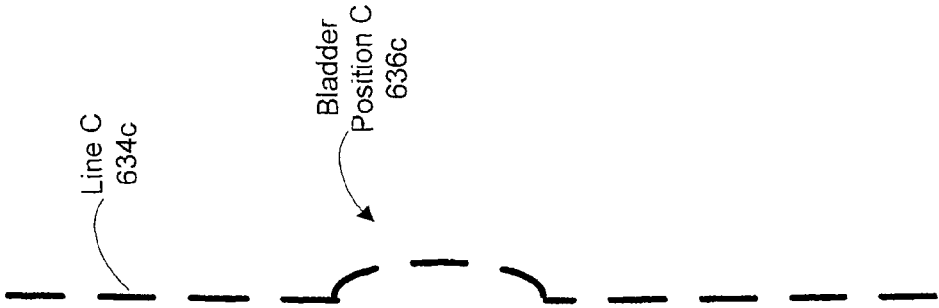


FIG. 6C

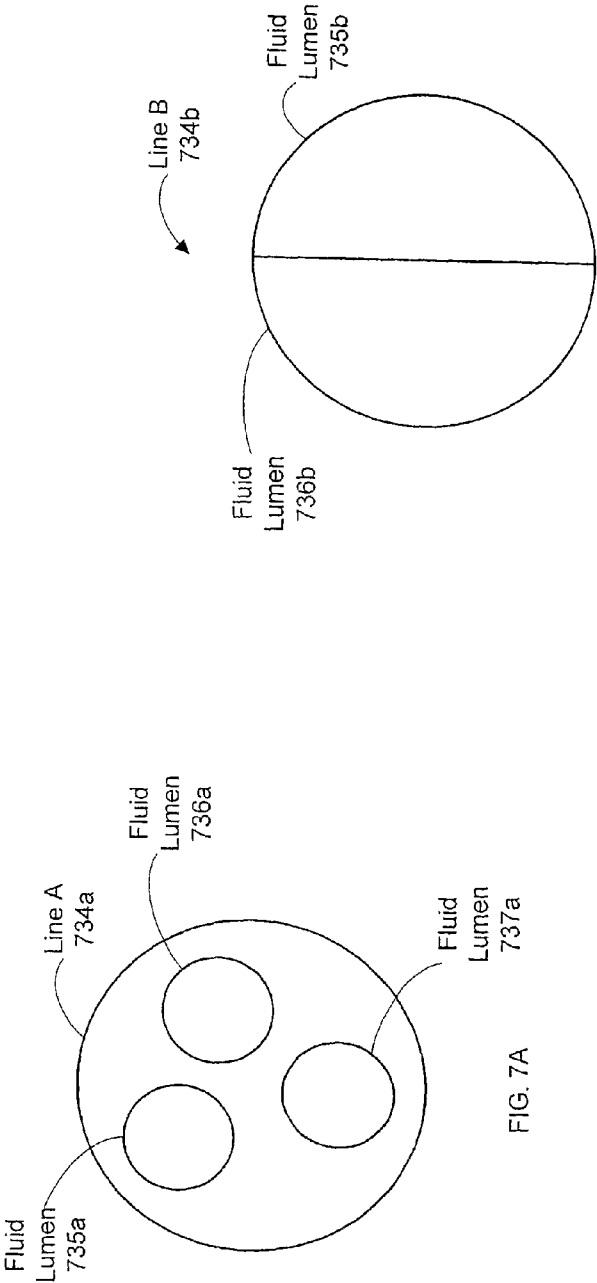


FIG. 7A

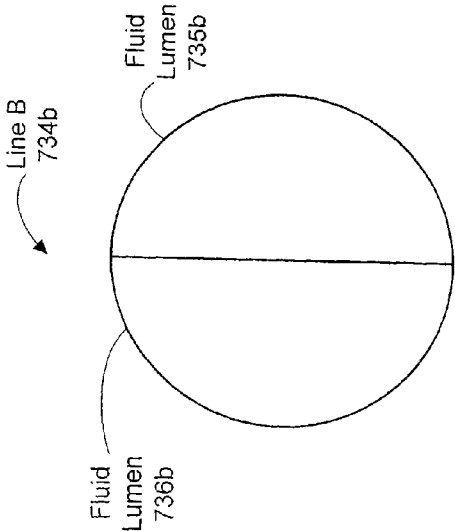


FIG. 7B

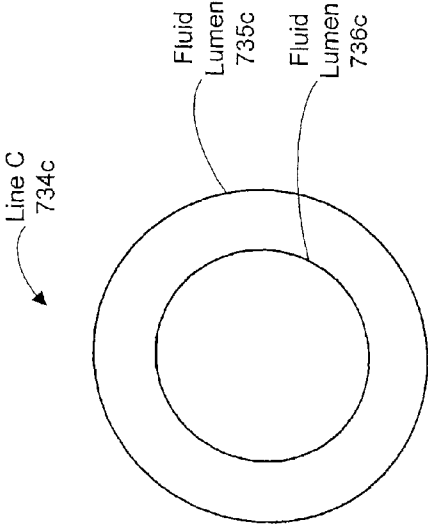


FIG. 7C

800

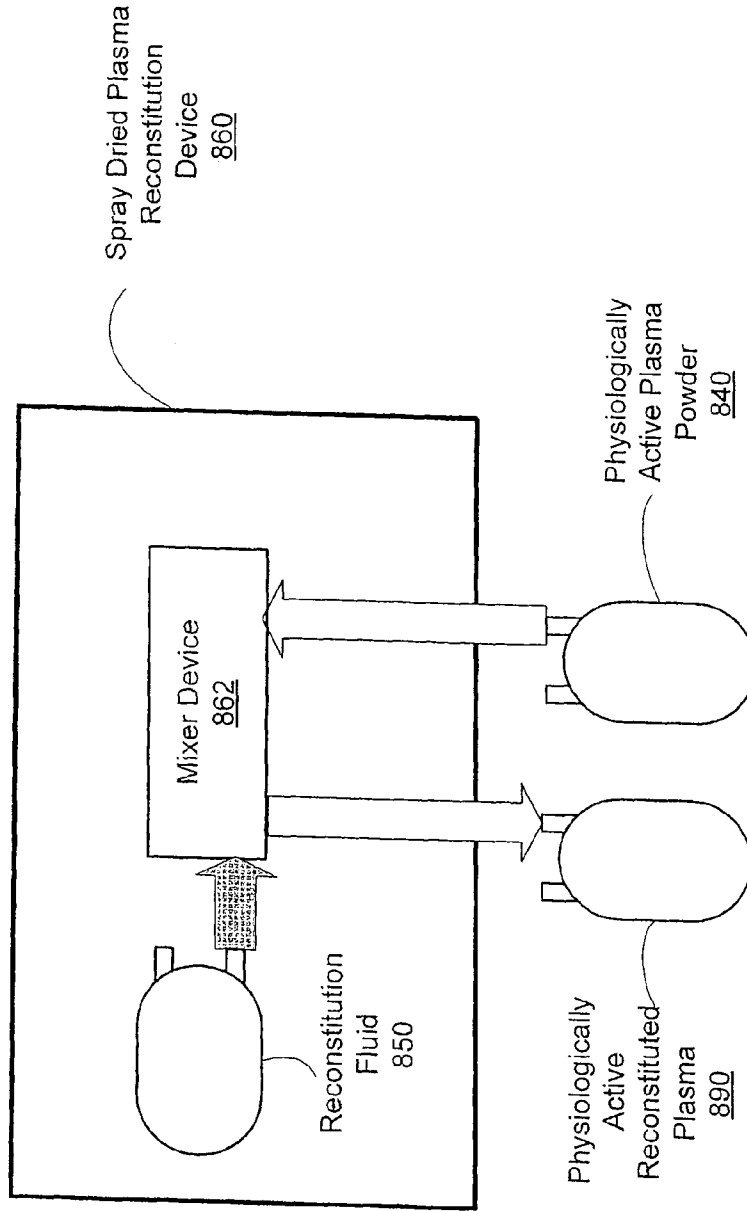
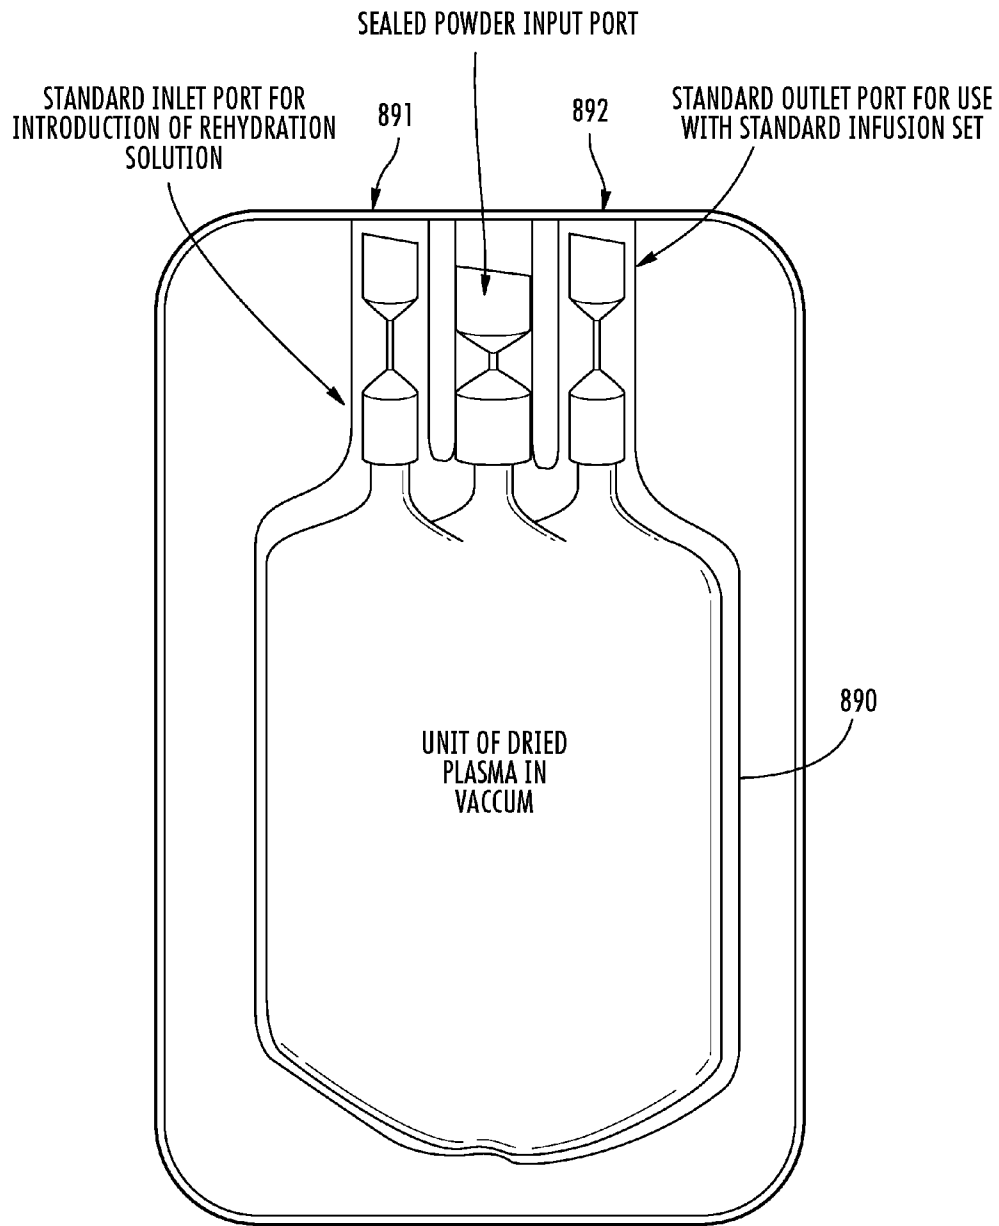


FIG. 8A



**FIG. 8B**



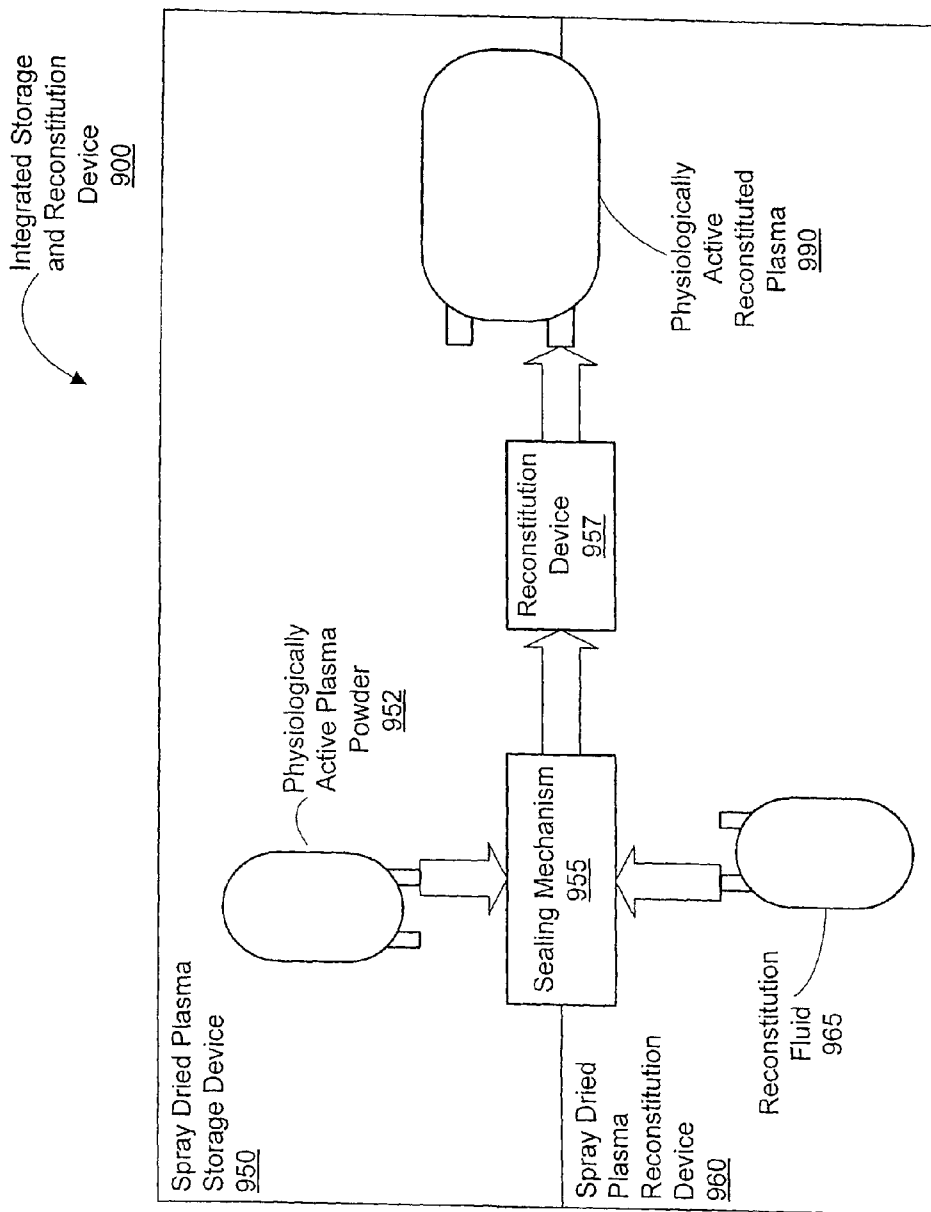
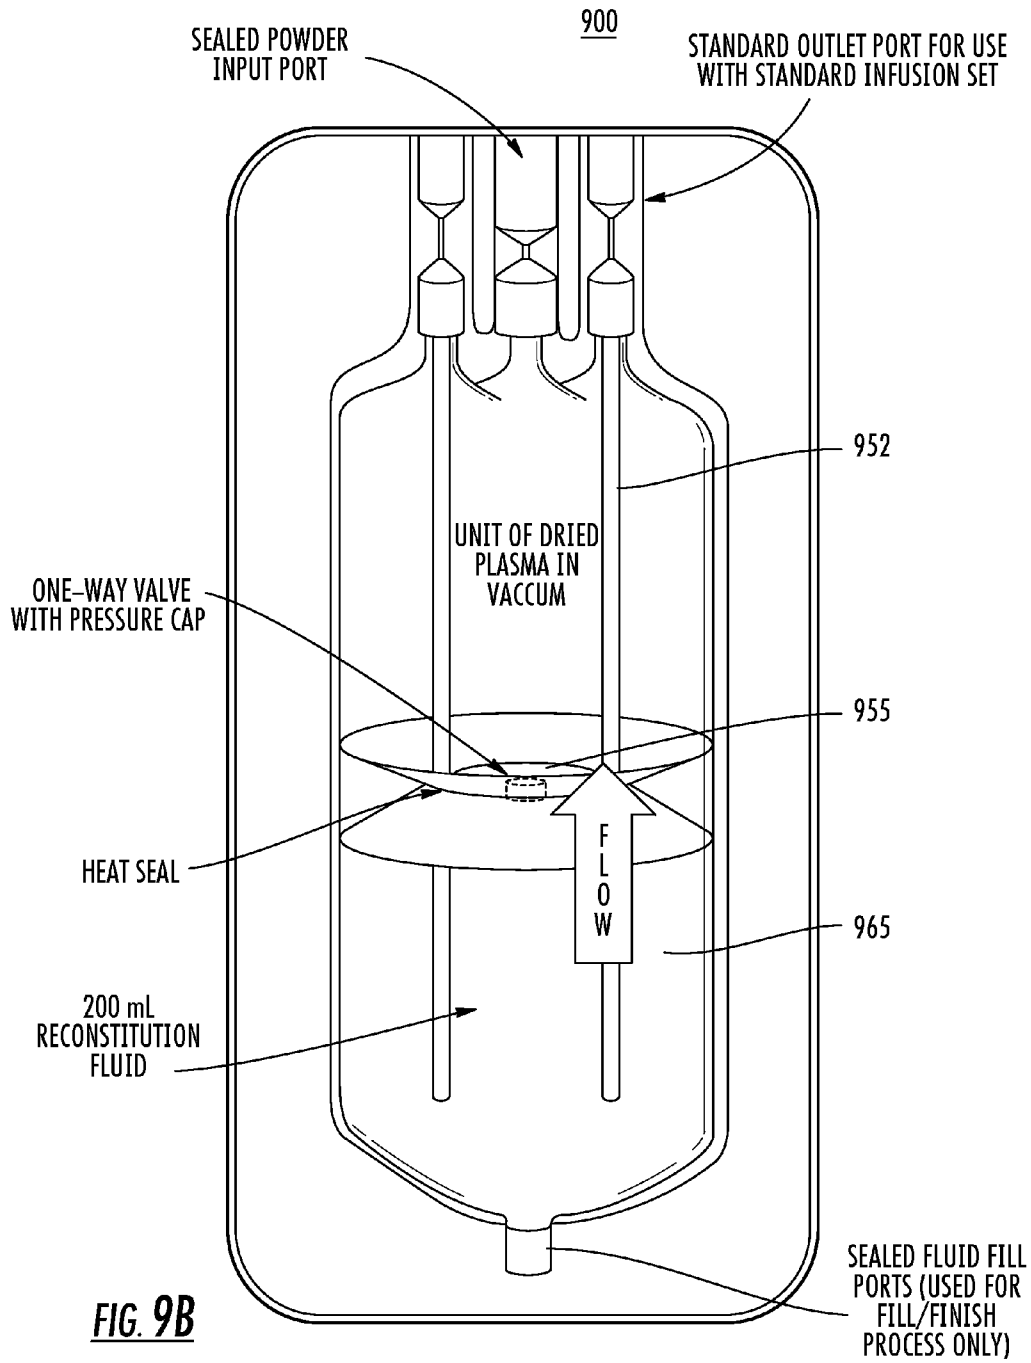


FIG. 9A



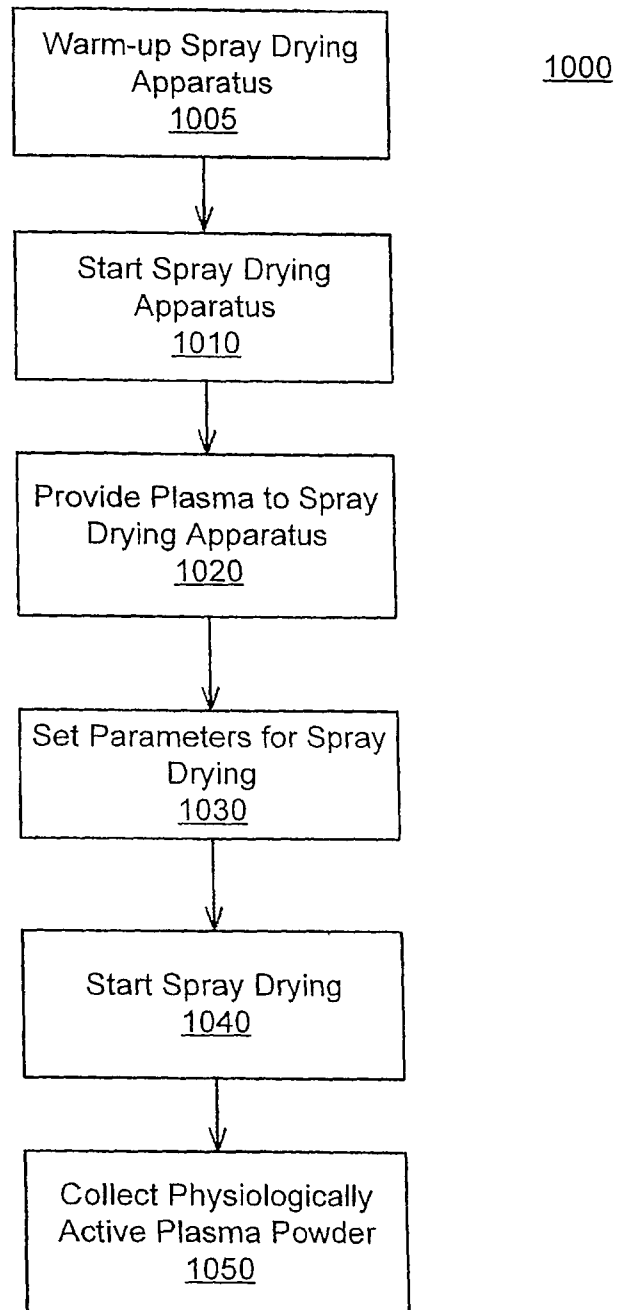


FIG. 10

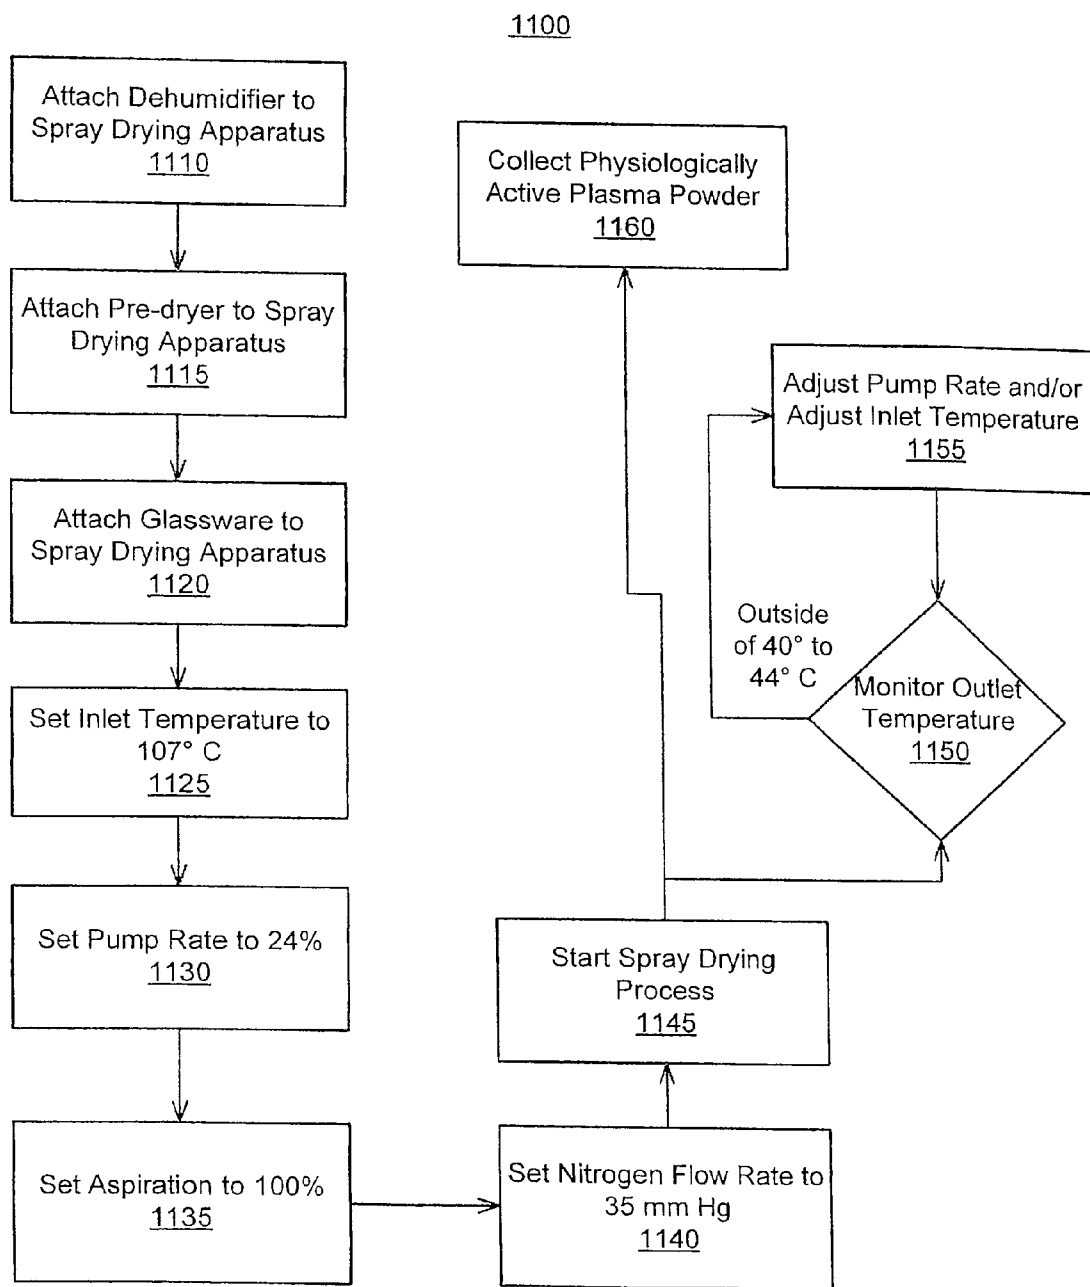


FIG. 11

1200

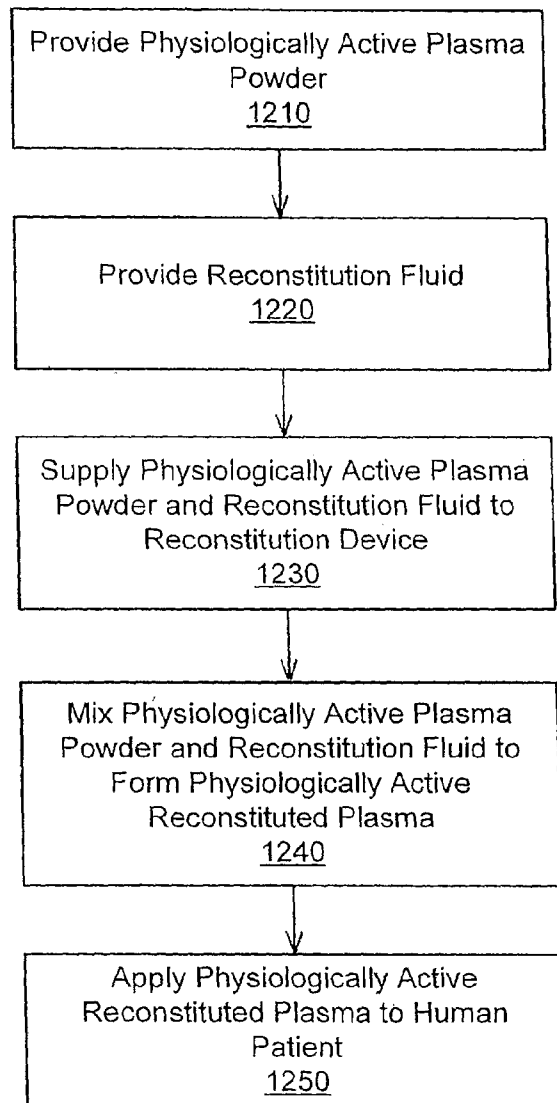
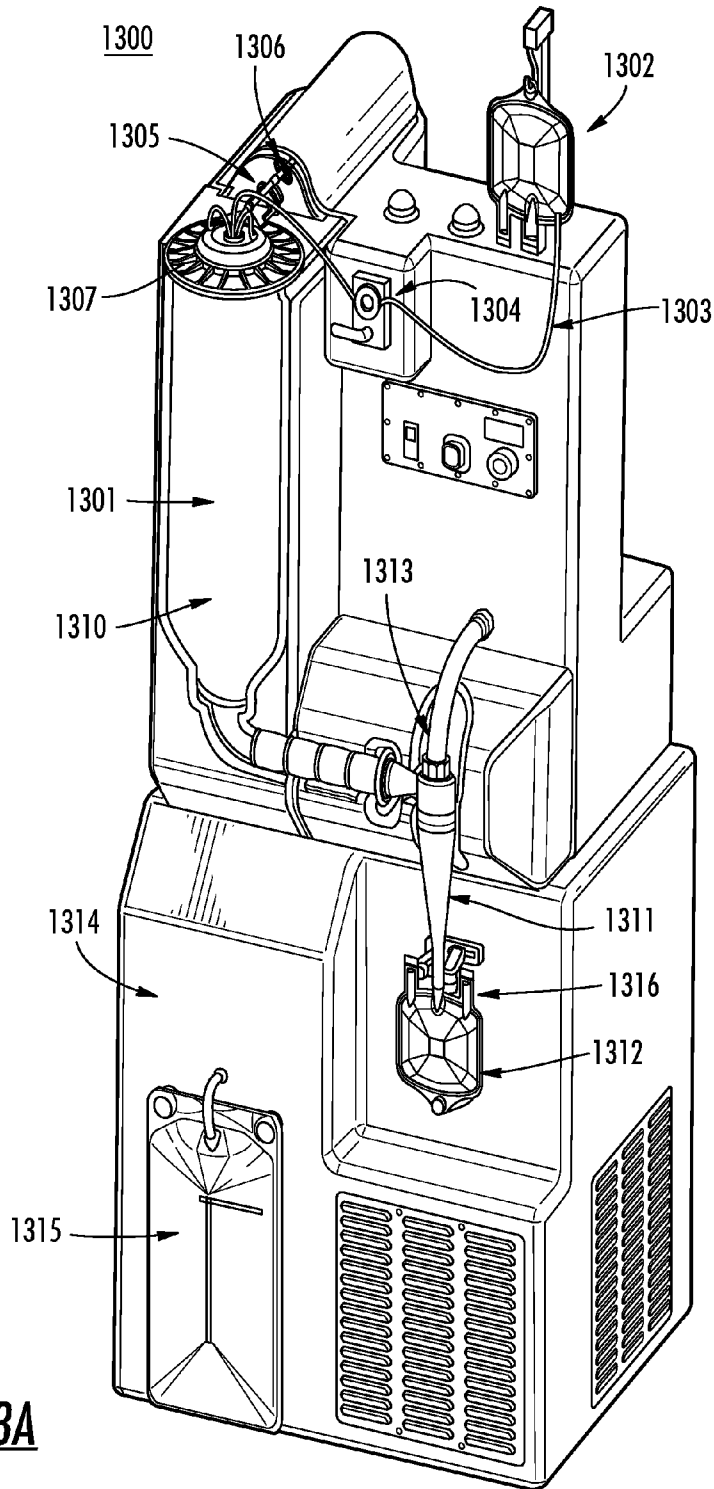


FIG. 12



**FIG. 13A**

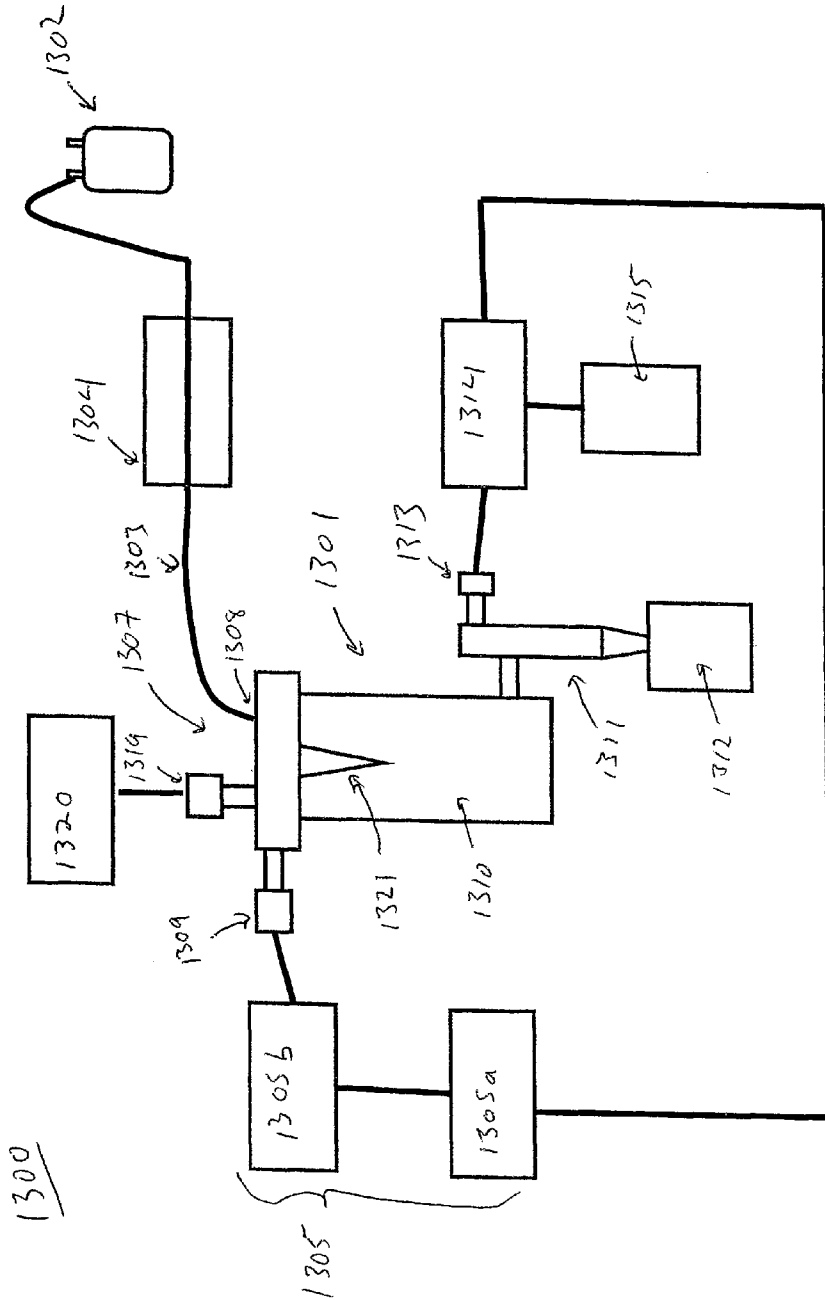


Fig. 13B

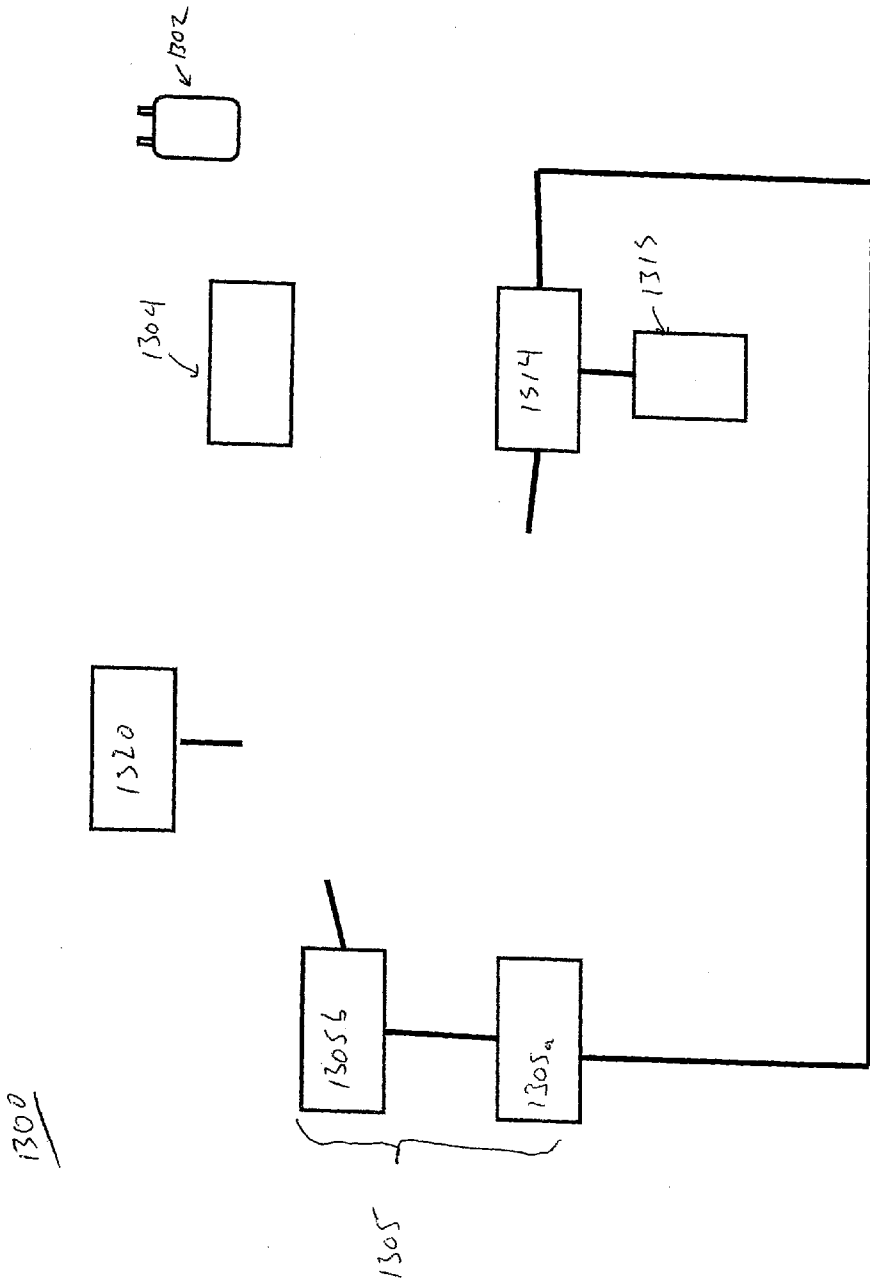


Fig. 13C



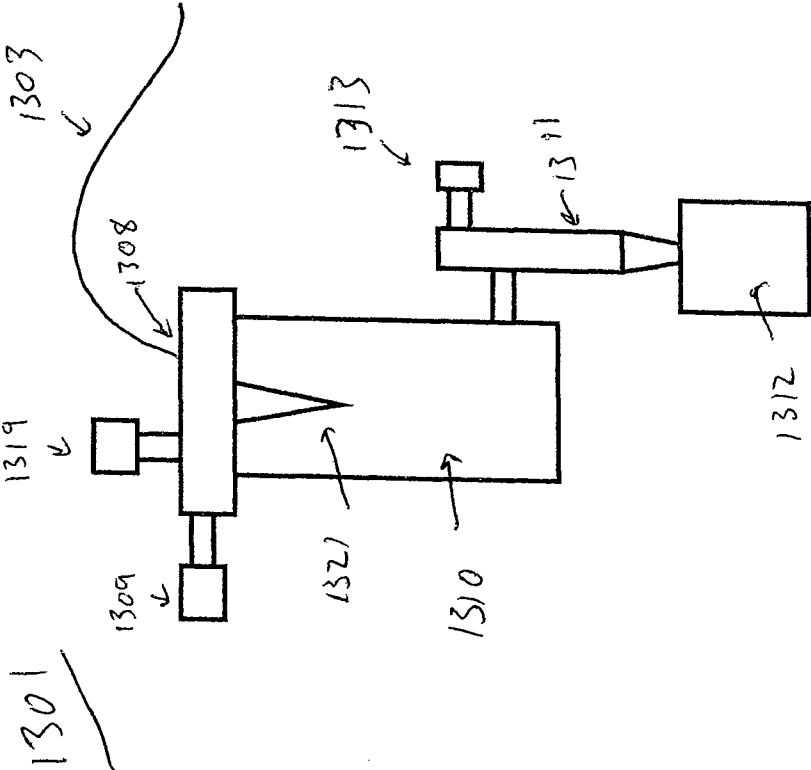
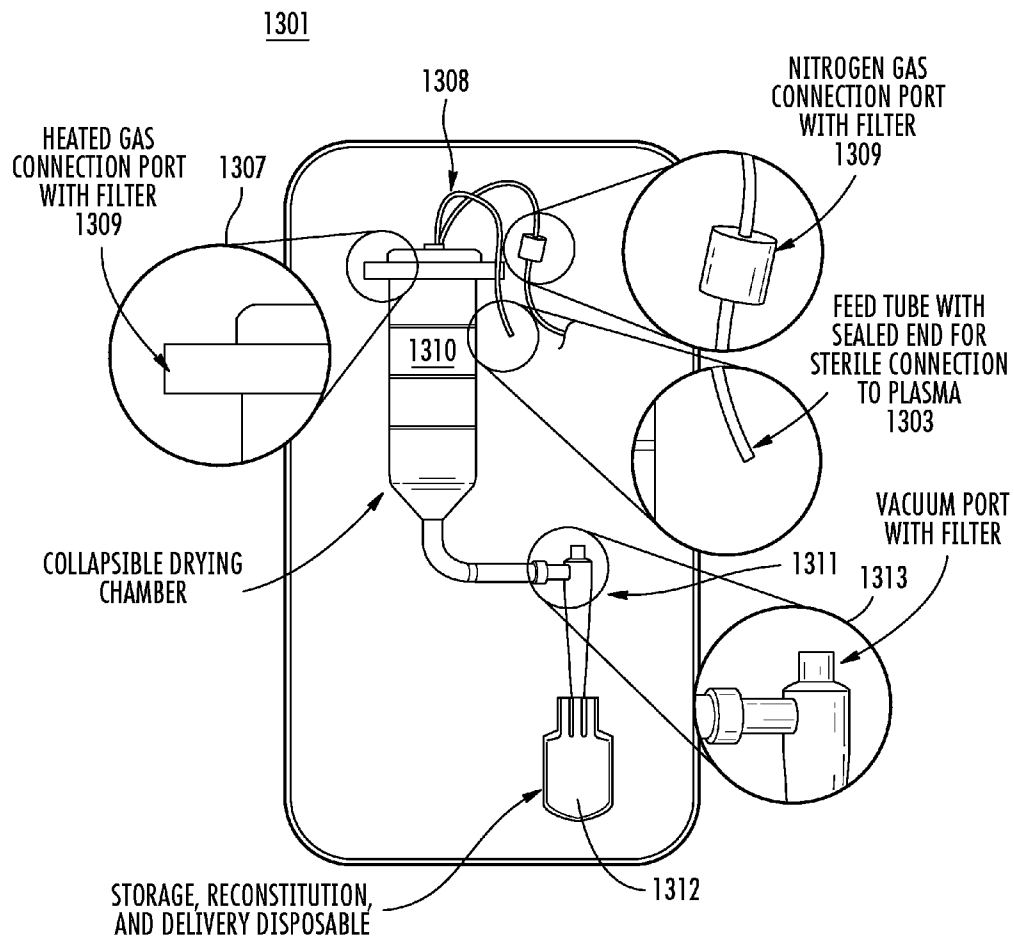
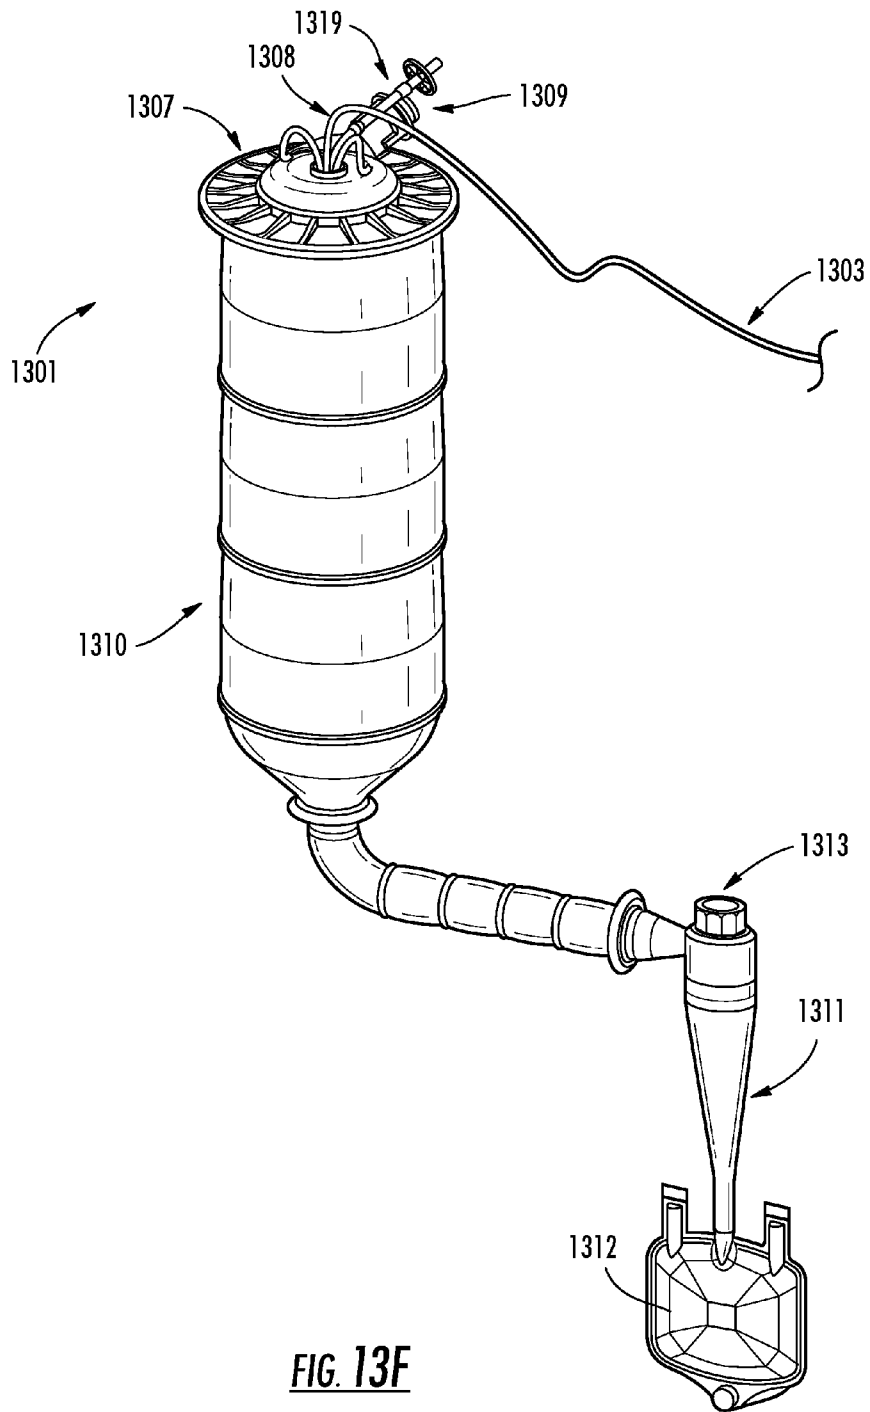


Fig. 13D



**FIG. 13E**



**FIG. 13F**

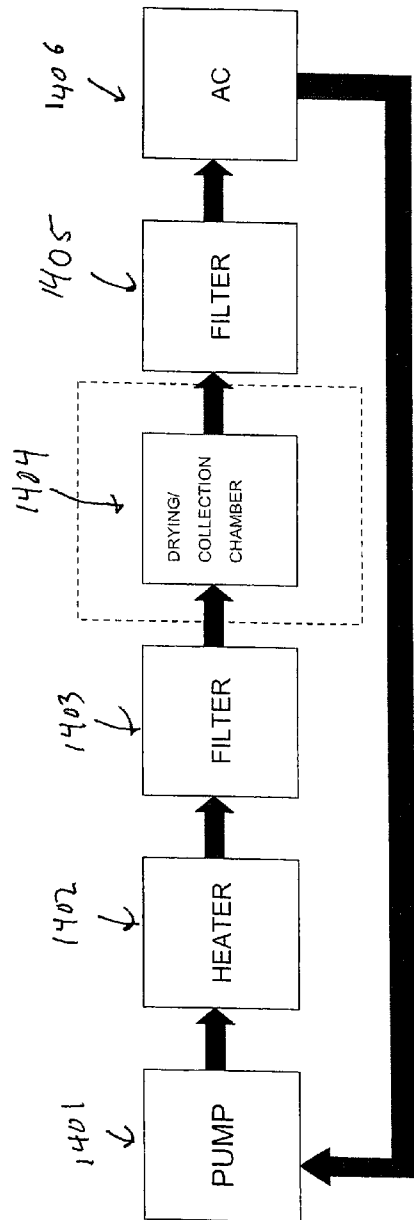


Fig. 14A


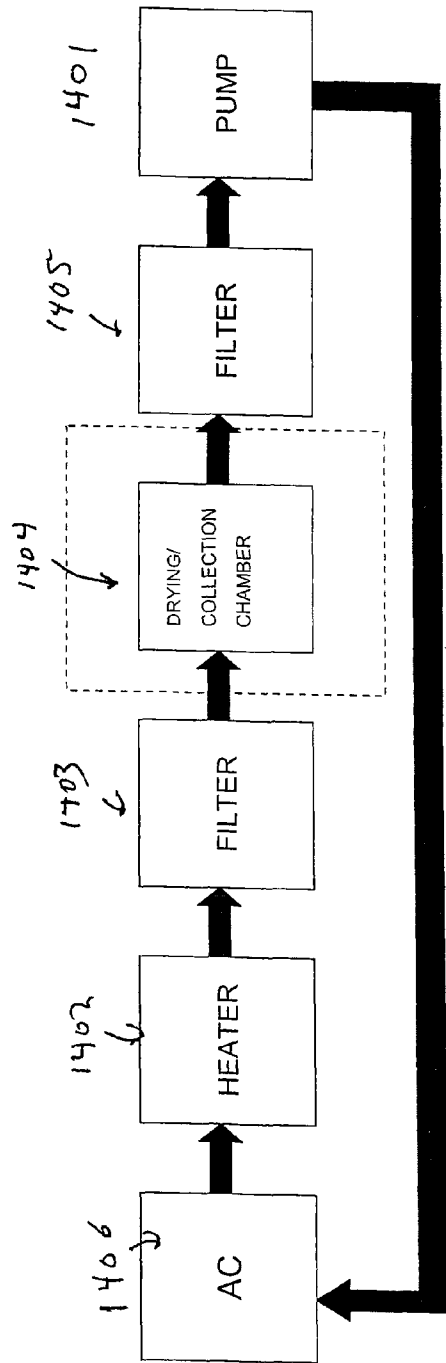


FIG. 14B

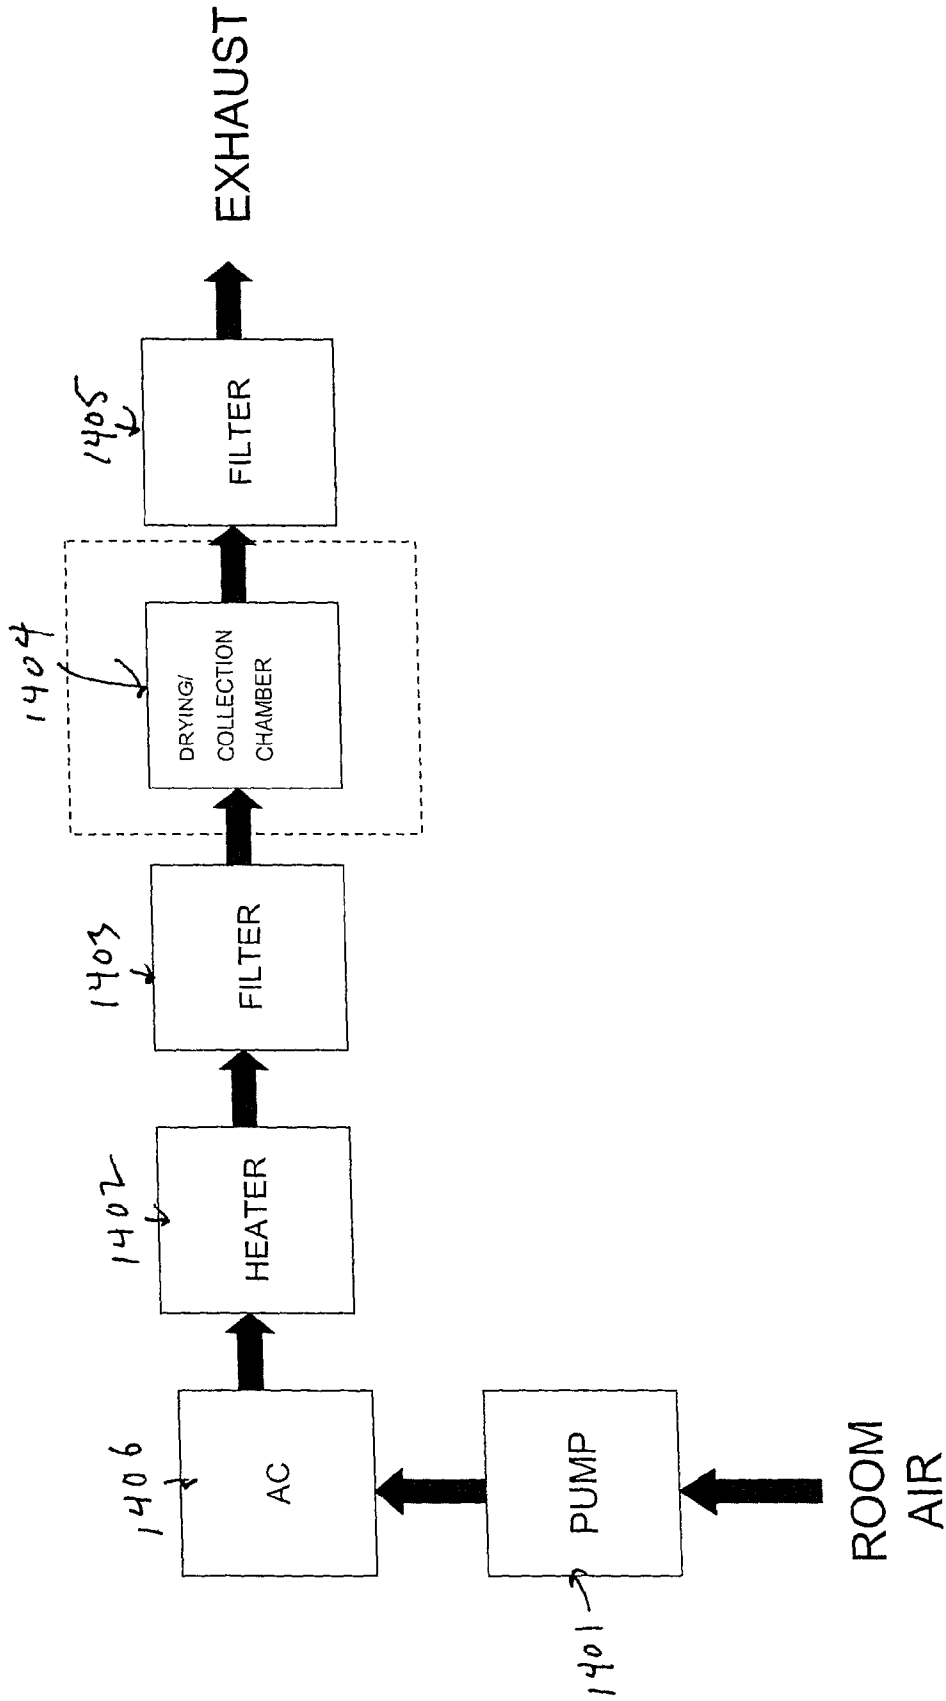

F.5 . 14C

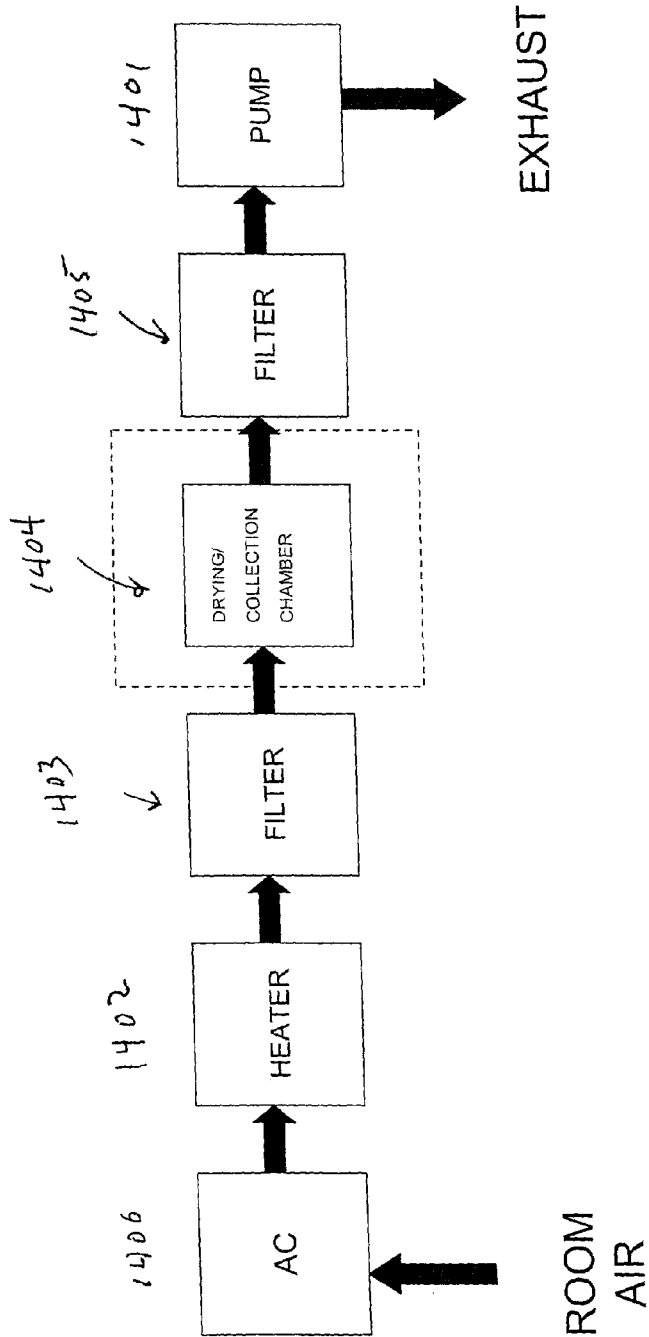


Fig. 14D

Coagulation Factor Activity of Thawed Plasma Derived from FFP\*

Coagulation Factor	Level †						Mean Change from Day 1 to Day 5 (%)	p Values
	Day 1	Day 2	Day 3	Day 4	Day 5	Day 5		
Factor VIII (%)	107 ± 26	76 ± 19	66 ± 18	65 ± 17	63 ± 16	41	<0.004†	
Blood group A	103 ± 44	74 ± 37	71 ± 35	67 ± 36	67 ± 33	35	<0.02†	
Blood group B	70 ± 16	51 ± 10	43 ± 10	43 ± 7	41 ± 8	41	<0.001†	
Blood group O	81 ± 9	81 ± 9	81 ± 9	80 ± 10	80 ± 10	1	NS	
Factor II (%)	79 ± 7	75 ± 8	71 ± 9	68 ± 9	66 ± 9	16	NS	
Factor V (%)	90 ± 18	81 ± 15	76 ± 15	72 ± 14	72 ± 15	20	NS	
Factor VII (%)	85 ± 13	84 ± 13	84 ± 15	82 ± 11	80 ± 11	6	NS	
Factor X	225 ± 12	224 ± 13	224 ± 13	224 ± 17	225 ± 12	0	NS	
Fibrinogen (mg/dL)								

FRS. 15



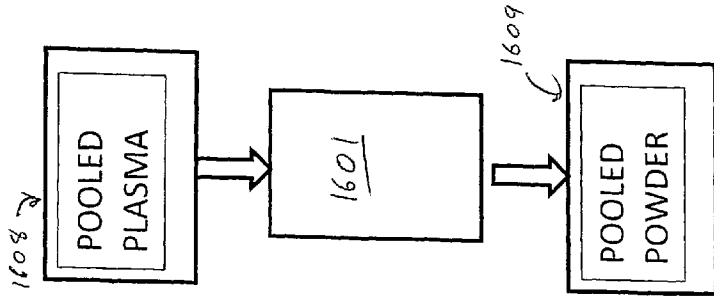


Fig. 16D

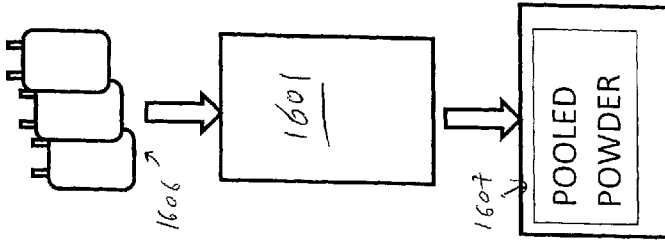


Fig. 16C

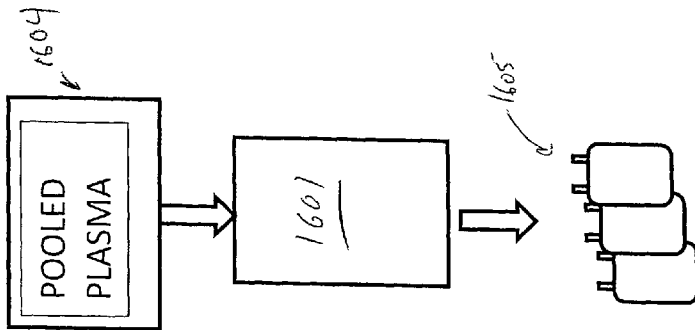


Fig. 16B

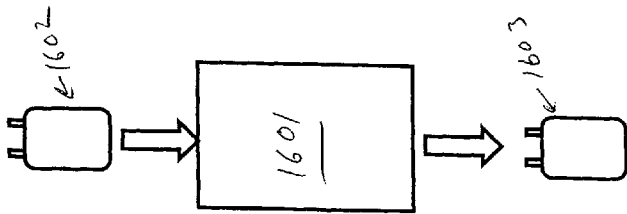


Fig. 16A

Characterization of Reconstituted Spray Dried Plasma

Settings		Samples Tested		Stago Test Results										
Inlet Temp	Feed Pump Setting			PT (sec)	aPTT (sec)	FNG (mg/dL)	F-5 (IU/dL)	F-7 (IU/dL)	F-8 (IU/dL)	F-9 (IU/dL)	PC Clot (IU/dL)	PS Clot (IU/dL)		
97 C	7%	6 For PT, aPTT, FNG		Average	27.5	46.6	186.8	73.0	96.5	68.0	121.0	128.0	93.0	
		1-2 For Factors and PS/PC		Min	14.1	28.1	64.0	38.0	82.0	49.0	106.0	128.0	88.0	
				Max	48.0	96.7	258.0	108.0	111.0	87.0	136.0	128.0	98.0	
97 C	Variable	1 For PT, aPTT, FIB		Average	22.5	46.4	216.3	43.0	60.0	42.5	66.8	92.5	66.0	
		2 for PS/PC		Min	19.2	37.2	109.0	17.0	40.0	23.0	49.0	89.0	64.0	
		(Minimum 6 for Factors)		Max	26.7	66.0	273.0	65.0	86.0	85.0	78.0	96.0	68.0	
112 C	Variable	34		Average	25.8	50.2	197.6	49.6	68.0	39.3	63.9	86.5	79.8	
		7 for PS/PC		Min	20.2	36.6	121.0	27.0	33.0	10.0	7.0	54.0	66.0	
				Max	42.2	97.1	292.0	73.0	93.0	89.0	107.0	104.0	111.0	
117 C	Variable	Minimum 10 For PT, aPTT, FIB		Average	27.3	56.5	187.2	41.8	72.5	32.3	65.3	88.3	63.3	
		2 for PS/PC		Min	21.9	48.7	129.0	31.0	31.0	9.0	13.0	59.0	56.0	
		Minimum 10 For Factors		Max	30.8	63.8	273.0	59.0	110.0	65.0	109.0	107.0	69.0	

FIG. 17A

Characterization of Reconstituted Spray Dried Plasma

Batch		Name	PT+ 10 (sec.)	aPTT (sec.)	FNG (mg/dL)	F-5 (IU/dL)	F-7 (IU/dL)	F-8 (IU/dL)	F-9 (IU/dL)
2010-040	1	2010-040GLY	17.2	41.6	259	93	81	96	108
2010-040	1	2010-040-GLY	14.4	40.2	281	107	95	14	16
2010-041	1	2010-041GLY	16.3	39.9	271	93	84	98	118
2010-072	1	2010-072GLY	14.4	34.7	277	105	80	46	116
2010-074	1	2010-074GLY	13.8	30.5	346	63	85	88	106
2010-077	1	2010-077GLY	15.9	32.2	360	88	64	84	96
2010-079	1	2010-079GLY	14.4	36.3	259	83	86	44	79
2010-081	1	2010-081GLY	15.4	35.1	243	82	82	64	92
2010-083	1	2010-083GLY	16.1	39.1	267	60	96	36	108
2010-102	1	2010-102GLY	15.4	36.2	283	71	44	42	55
2010-104	1	2010-104GLY	16.0	34.6	235	53	39	40	83
		Average	15	36	280	82	76	59	89
		Min	14	31	235	53	39	14	16
		Max	17	42	360	107	96	98	118

FIG. 17B

**SPRAY DRIED HUMAN PLASMA****CROSS REFERENCE TO RELATED APPLICATION**

This application is a continuation of U.S. patent application Ser. No. 13/415,440, filed Mar. 8, 2012, which is a continuation of International No. PCT/US2010/049176, filed Sep. 16, 2010, entitled, "Spray Dried Human Plasma", the entire contents of which are incorporated herein by reference.

**FIELD OF THE INVENTION**

The present invention relates generally to methods and apparatus for producing and/or using spray dried human plasma.

**BACKGROUND**

Blood plasma is the yellow liquid component of blood, in which the blood cells of whole blood would normally be suspended. Blood plasma makes up about 55% of the total blood volume. Blood plasma is mostly water (e.g., 90% by volume) and contains dissolved proteins, glucose, clotting factors, mineral ions, hormones, and/or carbon dioxide. Blood plasma is prepared by spinning a tube of fresh blood in a centrifuge until the blood cells fall to the bottom of the tube. The blood plasma is then poured or drawn off. Blood plasma is frequently frozen fresh for future uses. Although frozen plasma is the current standard of care, there are numerous problems with this technology. For example, the bag containing the frozen plasma become brittle and often gets damaged during storage or transportation. Maintaining frozen plasma at the appropriate temperature during storage and transportation is very expensive. It requires mechanical freezers to keep the frozen plasma at  $-18^{\circ}\text{C}$ . or lower. Shipping requires special shipping containers to maintain the frozen state and reduce breakage of the bag. Use of the frozen plasma is delayed by 30-45 minutes due to the thawing time. Moreover, the preparation for use requires trained staff and specialized thawing device in a regulated laboratory. Finally, fresh frozen plasma has a limited shelf life of 12 months at  $-18^{\circ}\text{C}$ . Once thawed, the frozen plasma must be used within 24 hours.

In an attempt to avoid the disadvantages of frozen plasma, some have freeze dried (i.e., lyophilized) plasma. However, the freeze drying process produces a product composed of large, irregular sized grains or particles. Such products can be difficult or impossible to reconstitute to a form suitable for administration to a patient. Furthermore, the freeze drying process requires transfer of the product from the lyophilizer to the final container, thus requiring post-processing sterility testing. The freeze drying process can only be done in batch mode; continuous processing is not possible with freeze drying. Moreover, manufacturing scale-up requires changes to the freeze drying process, and there are protein recovery issues at scale-up.

Accordingly, a need still exists in the field for plasma that may be stored in a wide range of environments without freezers or refrigerators, be available for use by first responders at the initial point of care, and can be transfused in minutes without the 30-45 minute delay associated with thawing of frozen plasma.

**SUMMARY OF THE INVENTION**

The present invention provides an extracorporeal sterile, closed plasma processing system, which can be used to pro-

duce a spray dried, physiologically active plasma powder product that has a long storage life at room temperature; that can easily be stored and shipped; that is versatile, durable and simple, and that can be easily and rapidly reconstituted and used at the point of care. The processing system of the present invention can produce spray dried plasma in either a batch (single unit) or a continuous (pooled units) process mode. The resulting plasma powder can be dried directly into the final, attached sterile container, which can later be rapidly and easily reconstituted to produce transfusion grade plasma. The spray dried powder can be stored at least 2-3 years at virtually any temperature (e.g.,  $-180^{\circ}\text{C}$ . to  $50^{\circ}\text{C}$ .). The costs associated with storage and shipping of the spray dried powder are significantly lower, because of its lighter weight and broader range of temperature tolerance compared to frozen plasma. At the point of care, the spray dried powder is rapidly reconstituted (30-120 seconds), avoiding the need for special equipment and trained staff. In contrast to frozen plasma, which takes 30-45 minutes to thaw and must be used within 24 hours, the spray dried plasma of the present invention avoids waste since the caregiver can rapidly prepares the amount of plasma required for a given patient, rather than trying to assess and predict the amount of plasma required and thawing sufficient plasma to meet this anticipated need.

One approach to spray dried human plasma is a method that includes providing plasma to a spray drying apparatus; spray drying the plasma, at the spray drying apparatus, to form physiologically active plasma powder, the spray drying apparatus configured utilizing one or more parameters; and storing the physiologically active plasma powder.

Another approach to spray dried human plasma is a spray drying apparatus. The spray drying apparatus includes a pump device configured to transport plasma from a liquid plasma storage device at a pump rate; a heated air stream device configured to deliver an air stream at an inlet temperature; a non reactive gas supply device configured to supply a non reactive gas at a flow rate; a spray nozzle configured to spray the plasma into a spray chamber utilizing the non reactive gas and the air stream; and a particle collection device configured to collect the sprayed dried plasma via a vacuum formed by a vacuum pump at an aspiration setting.

Another approach to spray dried human plasma is a method. The method includes providing a physiologically active plasma powder; providing a reconstitution fluid; and reconstituting physiologically active reconstituted plasma by mixing the physiologically active plasma powder and the reconstitution fluid.

Another approach to spray dried human plasma is a method. The method includes providing, from a non reactive gas supply to a spray nozzle, a non reactive gas at a flow rate; providing, from a dehumidifier to the spray nozzle, a heated air stream at an inlet temperature; providing, from a pump device to the spray nozzle, plasma at a pump setting; spraying, at the spray nozzle, the non reactive gas, the heated air stream, and the plasma into a spray chamber to form a physiologically active plasma powder, the heated air stream enabling transfer of moisture from the plasma to the heated air stream.

Another approach to spray dried human plasma is a spray dried physiologically active plasma powder. The spray dried physiologically active plasma powder is prepared by providing plasma to a spray drying apparatus; and spray drying, at the spray drying apparatus, the plasma to form the physiologically active plasma powder, the spray drying apparatus configured utilizing one or more parameters.

Another approach to spray dried human plasma is a physiologically active reconstituted plasma. The physiologically

active reconstituted plasma is prepared by providing plasma to a spray drying apparatus; spray drying, at the spray drying apparatus, the plasma to form physiologically active plasma powder, the spray drying apparatus configured utilizing one or more parameters; and reconstituting the physiologically active plasma powder utilizing a reconstitution fluid to form the physiologically active reconstituted plasma.

As mentioned above, the processing systems of the type described herein can be used to produce spray dried physiologically active plasma powder in either a batch (single unit) or a continuous (pooled units) process mode.

One approach to spray dried human plasma is a method that starts with one unit of plasma and produces spray dried physiologically active plasma powder from that same unit of plasma. One advantage of this approach is that it allows the coding of the plasma unit, which permits tracking and removal of a particular plasma unit from circulation if an issue (e.g., infection, contamination) is subsequently identified with the original donor.

Another approach to spray dried human plasma is a method that starts with two or more single units of plasma and produces a pooled spray dried physiologically active plasma powder from these specific units of plasma. In addition to the ability to track the resulting product, another advantage of this approach is that the pooled powder can be reconstituted in a smaller volume to produce a high potency plasma unit. For example, if two units of plasma are spray dried and later reconstituted in one volume of reconstitution fluid, the resulting plasma would contain twice the concentration of physiologically active proteins, clotting factors, etc.

Yet another approach to spray dried human plasma is a method that starts with a pooled source of plasma containing two or more pooled single units of plasma and produces a series of single units of spray dried physiologically active plasma powder. This approach offers the efficiency advantages of a continuous processing mode to produce numerous single units of spray dried physiologically active plasma powder.

Yet another approach to spray dried human plasma is a method that starts with a pooled source of plasma containing two or more pooled single units of plasma and produces a pooled amount of spray dried physiologically active plasma powder. This approach offers the efficiency advantages of a continuous processing mode. This approach could be used, for example, to produce larger amounts of spray dried physiologically active plasma powder to be applied directly to an open wound.

In other embodiments, any of the approaches above can include one or more of the following features.

In one aspect, a method is disclosed for spray drying plasma, the method including: providing plasma to a spray drying apparatus; spray drying, at the spray drying apparatus, the plasma to form physiologically active plasma powder; and storing the physiologically active plasma powder.

Some embodiments include, during the providing, spray drying, and storing steps, maintaining the plasma and plasma powder in an isolated sterile environment. Some embodiments include, processing plasma in a closed sterile process to produce physiologically active plasma powder suitable for reconstitution and transfusion to a human subject.

Some embodiments include, during the spray drying, maintaining the plasma at a temperature below a threshold temperature to prevent denaturing of proteins in the plasma. In some embodiments, the threshold temperature is 44° C. or less. In some embodiments, the threshold temperature is 48° C. or less. In some embodiments, the threshold temperature is 50° C. or less.

Some embodiments include, during the spray drying, maintaining the plasma at a temperature within a selected temperature range. Some embodiments include during the spray drying, maintaining the plasma at a temperature within a selected temperature range of 41-43° C. or 37-48° C.

In some embodiments, spray drying the plasma includes: directing plasma to a spray nozzle at a plasma flow rate; directing a heated drying gas to a drying chamber at an inlet temperature and a drying gas flow rate; directing a non reactive spray gas to the nozzle at a spray gas flow rate; combing the plasma and spray gas at the nozzle to atomize the plasma and dry the plasma; and combining the atomized plasma and drying gas to dry the atomized plasma.

In some embodiments, the inlet temperature is in the range of 85-120° C. or 92-117° C.

In some embodiments, the plasma flow rate is in the range of 2-20 mL/minute, 2-30 mL/min, 2-50 mL/min, etc. In some embodiments, the drying gas flow rate is in the range of 20-80 m<sup>3</sup>/hour. In some embodiments, the spray gas flow rate is in the range of 300-500 L/hr.

In some embodiments, the plasma flow rate is in the range of 8-12 mL/minute. In some embodiments, the drying gas flow rate is in the range of 30-40 m<sup>3</sup>/hour. In some embodiments, and the spray gas flow rate is in the range of 350-450 L/hr.

Some embodiments include determining an outlet temperature of the plasma powder; and adjusting at least one of: the plasma flow rate, the inlet temperature, the spray gas flow rate, and the drying gas flow rate based on the outlet temperature.

Some embodiments include reconstituting the physiologically active plasma powder utilizing a reconstitution fluid to form physiologically active reconstituted plasma.

Some embodiments include applying the physiologically active reconstituted plasma to a human. In some embodiments, the reconstitution fluid includes at least one selected from the list consisting of: distilled water, saline solution, and glycine. In some embodiments, the reconstitution fluid is a buffered solution.

In some embodiments, the powder, when reconstituted, exhibits physiological activity substantially equivalent to Thawed Plasma, Liquid Plasma, FP24, or FFP.

In some embodiments, the dried plasma, when reconstituted, is characterized by an aPTT of about 65 seconds or less, a PT of about 31 seconds or less, and a Fibrinogen level of at least about 100 mg/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by an aPTT of about 35 seconds or less, a PT of about 15 seconds or less, and a Fibrinogen level of at least about 223 mg/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by an aPTT in the range of 28-66 seconds, a PT in the range of 14-31 seconds, and a Fibrinogen level in the range of 100-300 mg/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by an aPTT in the range of 30-35 seconds, a PT in the range of 10-15 seconds, and a Fibrinogen level in the range of 223-500 mg/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level of at least about 10 IU/dL, a Factor IX level of at least about 10 IU/dL, a Protein C level of at least about 10 IU/dL, and a Protein S level of at least about IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level of at least about 30 IU/dL, a Factor IX level of at least about

IU/dL, a Protein C level of at least about 55 IU/dL, and a Protein S level of at least about 54 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level of at least about 54 IU/dL, a Factor IX level of at least about 70 IU/dL, a Protein C level of at least about 74 IU/dL, and a Protein S level of at least about 61 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level in the range of 30-110 IU/dL, a Factor IX level in the range of 25-135 IU/dL, a Protein C level in the range of 55-130 IU/dL, and a Protein S level of in the range of 55-110 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level in the range of 34-172 IU/dL, a Factor IX level in the range of 70-141 IU/dL, a Protein C level in the range of 74-154 IU/dL, and a Protein S level of in the range of 61-138 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor V level of at least about 10 IU/dL, and a Factor VIII level of at least about 10 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor V level of at least about 30 IU/dL, and a Factor VIII level of at least about 25 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor V level of at least about 63 IU/dL, and a Factor VIII level of at least about 47 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of a Factor V level in the range of 63-135 IU/dL, a Factor VIII level in the range of 47-195 IU/dL.

In some embodiments, the powder has an average particle size of about 30 microns or less. In some embodiments, the powder has a maximum particle size of about 100 microns or less.

In some embodiments, the powder includes at least 30% dried protein by weight.

In some embodiments, when reconstituted with 1 mL of fluid per 0.09 grams of powder, the reconstituted plasma has a protein concentration in the range of 35 mg/mL to 60 mg/mL.

In another aspect, a product is disclosed including: a physiologically active dried plasma in the form of a powder. In some embodiments, the physiologically active dried plasma is sterile.

In some embodiments, the powder, when reconstituted, exhibits physiological activity substantially equivalent to Thawed Plasma, Liquid Plasma, FP24, or FFP.

In some embodiments, the dried plasma, when reconstituted, is characterized by an aPTT of about 65 seconds or less, a PT of about 31 seconds or less, and a Fibrinogen level of at least about 100 mg/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by an aPTT of about 35 seconds or less, a PT of about 15 seconds or less, and a Fibrinogen level of at least about 223 mg/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by an aPTT in the range of 28-66 seconds, a PT in the range of 14-31 seconds, and a Fibrinogen level in the range of 100-300 mg/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by an aPTT in the range of 30-35 seconds, a PT in the range of 10-15 seconds, and a Fibrinogen level in the range of 223-500 mg/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level of at least about 10 IU/dL, a Factor IX level of at least about 10 IU/dL, a Protein C level of at least about 10 IU/dL, and a Protein S level of at least about 10 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level of at least about 30 IU/dL, a Factor IX level of at least about 25 IU/dL, a Protein C level of at least about 55 IU/dL, and a Protein S level of at least about 54 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level of at least about 54 IU/dL, a Factor IX level of at least about 70 IU/dL, a Protein C level of at least about 74 IU/dL, and a Protein S level of at least about 61 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level in the range of 30-110 IU/dL, a Factor IX level in the range of 25-135 IU/dL, a Protein C level in the range of 55-130 IU/dL, and a Protein S level of in the range of 55-110 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor VII level in the range of 34-172 IU/dL, a Factor IX level in the range of 70-141 IU/dL, a Protein C level in the range of 74-154 IU/dL, and a Protein S level of in the range of 61-138 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor V level of at least about 10 IU/dL, and a Factor VIII level of at least about 10 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor V level of at least about 30 IU/dL, and a Factor VIII level of at least about 25 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of: a Factor V level of at least about 63 IU/dL, and a Factor VIII level of at least about 47 IU/dL.

In some embodiments, the dried plasma, when reconstituted, is characterized by at least one of a Factor V level in the range of 63-135 IU/dL, a Factor VIII level in the range of 47-195 IU/dL.

In some embodiments, the powder has an average particle size of about 30 microns or less. In some embodiments, the powder has a maximum particle size of about 100 microns or less.

In some embodiments, the powder includes at least 30% dried protein by weight.

In some embodiments, when reconstituted with 1 mL of fluid per 0.09 grams of powder, the reconstituted plasma has a protein concentration in the range of 35 mg/mL to 60 mg/mL.

In another aspect, an apparatus is disclosed for spray drying plasma including: a plasma source; a pressurized spray gas source; a drying gas source; a spray dry nozzle in sterile fluid communication with the plasma and spray gas sources; a drying chamber in fluid communication with the spray dry nozzle and the drying gas source to receive a spray of plasma from the nozzle for drying; a particle collection device configured to collect spray dried plasma from an outlet of the drying chamber; and a collection device gas outlet port in sterile fluid communication with the collection device, the gas outlet port including a sterile outlet port. In some embodiments, the spray nozzle, drying chamber, and collection device define a sterile isolated interior volume.

In some embodiments, the gas outlet port includes a sterile filter.

In some embodiments, the nozzle is in sterile fluid communication with each of the spray gas source and the drying gas source through a respective sterile filter.

In some embodiments, the gas outlet port is in fluid communication with an external volume through the sterile outlet filter.

In some embodiments, the gas outlet port is in fluid communication with the drying gas source to provide closed recirculation of the drying gas.

In some embodiments, the plasma source includes a peristaltic pump configured to deliver a flow of plasma to an inlet of the nozzle at a plasma flow rate.

In some embodiments, the spray gas source includes a source of pressurized non reactive gas, and is configured to deliver the non reactive gas to the nozzle at a spray gas flow rate.

In some embodiments, the drying gas source includes a source of drying gas, and is configured to deliver heated drying gas to the nozzle at a drying gas flow rate and an inlet temperature.

Some embodiments include a controller configured to control at least one selected from the list consisting of: the plasma flow rate, the spray gas flow rate, the drying gas flow rate, and the inlet temperature.

In some embodiments, at least one sensor for measuring outlet temperature information indicative of an outlet temperature the spray dried plasma, the sensor in communication with the controller. In some embodiments, the controller includes a servo loop that controls the outlet temperature to a selected value by adjusting, based on the outlet temperature information, at least one selected from the list consisting of: the plasma flow rate, the spray gas flow rate, the drying gas flow rate, and the inlet temperature. In some embodiments, the controller includes a servo loop that controls the outlet temperature to a selected value by adjusting, based on the outlet temperature information, the plasma flow rate.

In another aspect, an attachment for plasma spray drying apparatus including: a plasma inlet port for sterile attachment to a plasma source; a spray gas inlet port for removable sterile attachment to a pressurized gas source; at least one drying gas inlet port for removable sterile attachment to a drying gas source; a spray dry nozzle in fluid communication with the plasma and spray gas inlets; a drying chamber in fluid communication with the attached spray nozzle and drying gas inlet to receive a spray of plasma for drying; a particle collection device configured to collect spray dried plasma from an outlet of the drying chamber; and a collection device gas outlet port in sterile fluid communication with the collection device. In some embodiments, the spray nozzle, drying chamber, and collection device define a sterile isolated interior volume.

In some embodiments, at least one of the inlet and outlet ports includes a sterile filter.

In some embodiments, the drying chamber is at least partially collapsible.

In some embodiments, the attachment includes a plastic or polymer material.

In some embodiments, the particle collection device includes a cyclone chamber.

In some embodiments, the particle collection device includes a detachable storage portion configured to receive collected spray dried plasma.

In another aspect, a product is disclosed including: a physiologically active spray dried plasma powder made using the methods described herein, e.g., the method described above.

Various embodiments may include any of the above described features, techniques, elements, etc., either alone, or in any suitable combination.

The plasma spray drying techniques described herein can provide one or more of the following advantages. An advantage to the plasma spray drying techniques described herein is that the plasma is not overheated during the spray drying process, which increases the recovery rate of physiologically functional plasma proteins, thereby increasing the efficacy of the plasma powder. Another advantage to the plasma spray drying techniques described herein is that the plasma can be stored for future use without refrigeration, thereby extending the shelf life and potential uses of the plasma (e.g., on the battlefield, in space, at sea, etc.). An additional advantage to the plasma spray drying techniques described herein is that the process parameters are controlled by the output temperature thereby enabling the quantity of processed plasma to be scaled by monitoring the output temperature and adjusting the pump rate and/or the inlet temperature accordingly to meet the required output temperature for the spray dried plasma.

Other aspects and advantages of the present invention will become apparent from the following detailed description, taken in conjunction with the accompanying drawings, illustrating the principles of the invention by way of example only.

#### BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other objects, features, and advantages of the present invention, as well as the invention itself, will be more fully understood from the following description of various embodiments, when read together with the accompanying drawings.

FIGS. 1A-1B are diagrams of exemplary spray drying systems;

FIG. 2 is a diagram of another exemplary spray drying system;

FIG. 3A is a diagram of another exemplary spray drying system;

FIG. 3B is an illustration of a cyclone chamber;

FIGS. 4A-4C are diagrams of exemplary spray nozzles;

FIGS. 5A-5B are diagrams of other exemplary centrifuge systems;

FIGS. 6A-6C are diagrams of exemplary bladder positions for centrifuge devices;

FIGS. 7A-7C are diagrams of exemplary lines for centrifuge devices;

FIG. 8A is a diagram of an exemplary spray dried plasma reconstitution device;

FIG. 8B is a diagram of an exemplary spray dried plasma storage bag;

FIG. 9A is a diagram of an exemplary integrated storage and reconstitution device;

FIG. 9B is a diagram of an exemplary integrated storage and reconstitution device;

FIG. 10 is a flowchart depicting an exemplary spray drying process for plasma;

FIG. 11 is a flowchart depicting another exemplary spray drying process for plasma;

FIG. 12 is a flowchart depicting an exemplary process of applying physiologically active reconstituted plasma to a human patient;

FIG. 13A-13C are diagrams of another exemplary spray drying system;

FIGS. 13D-13F are diagrams of an attachment to a spray drying system;

FIGS. 14A-D are illustrations of air flow configurations for various spray drying systems;

FIG. 15 is a chart illustrating the physiological activity of fresh frozen plasma, with the following symbol definitions: \*from Downes et al. "Serial measurement of clotting factors in thawed plasma for five days." *Transfusion* 2001; 41:570; †Mean±SD; ‡Comparison of Factor VIII activity at Day 1 and that at Day 3 was statistically significant;

FIGS. 16A-16D are diagrams illustrating spray dry batch process procedures;

FIGS. 17A-17B are charts illustrating the results of tests on spray dried plasma.

#### DETAILED DESCRIPTION

The spray drying system can be utilized to produce physiologically active plasma powder from human plasma. The spray drying system can dry the human plasma to form the physiologically active plasma powder while not overheating the human plasma which causes proteins within the human plasma to lose their efficacy (i.e., denatures the proteins). The spray drying system can utilize a heating source to heat the human plasma via a heated air stream. The heating of the human plasma via the heated air stream can remove the moisture from the human plasma while not denaturing the proteins within the human plasma thereby increasing the efficacy of the physiologically active plasma powder. For example, in some embodiments the moisture is removed by evaporative processes only, and not boiling.

The spray drying system can dry human plasma in a sterile, isolated environment. That is, during the spray drying process, the human plasma and resulting dried plasma powder can be kept isolated from any non sterile contaminants. Accordingly, the dried plasma powder product can be stored for time periods of months or more without the possibility of the growth of, e.g., bacterial contaminants.

As used herein, the term physiologically active plasma powder refers to any plasma powder which, when reconstituted, includes proteins that have not been damaged to such an extent to lose substantially all of their physiological efficacy. The physiological activity of a plasma powder, in its reconstituted form, may be indicated by a number of parameters known in the art including, but not limited to: Prothrombin Time (PT), Activated Partial Thromboplastin Time (aPTT), Fibrinogen level, Protein C level, and Protein S level. The physiological activity of a plasma powder, in its reconstituted form, may be indicated by coagulation factor levels known in the art including, but not limited to: Factor II, Factor V, Factor VII, Factor VIII, Factor IX, and Factor X. These parameters may be measured using techniques known in the art, e.g., using instruments available from DIAGNOSTICA STAGO, Inc. of Five Century Drive Parsippany, N.J., 07054.

Devices and techniques described herein may be used to produce plasma powder which, when reconstituted, has substantially the same level of physiological activity as, e.g., native plasma, fresh frozen plasma (FFP), or plasma frozen within 24 hours of phlebotomy (FP24), Thawed Plasma, or Liquid Plasma.

For example, as set forth in the Circular of Information For The Use of Human Blood Components (August 2009, available online at <http://www.aabb.org/resources/bct/Documents/coi0809r.pdf>) prepared jointly by the Advancing Transfusion and Cellular Therapies Worldwide (AABB), the American Red Cross, America's Blood Centers, and the Armed Services Blood Program (ASBP), FFP is prepared

for use for the relevant blood collection, processing, and storage system (e.g., frozen within eight hours of draw). On average, units contain 200 to 250 mL, but apheresis derived units may contain as much as 400 to 600 mL. FFP contains plasma proteins including all coagulation factors. FFP contains high levels of the labile coagulation Factors V and VIII. FFP should be infused immediately after thawing or stored at 1 to 6° C. for up to 24 hours. If stored longer than 24 hours, the component must be relabeled or discarded depending on the method of collection. FFP serves as a source of plasma proteins for patients who are deficient in or have defective plasma proteins.

FP24 is prepared from a whole blood collection and must be separated and placed at -18° C. or below within 24 hours from whole blood collection. The anticoagulant solution used and the component volume are indicated on the label. On average, units contain 200 to 250 mL. This plasma component is a source of non labile plasma proteins. Levels of Factor VIII are significantly reduced and levels of Factor V and other labile plasma proteins are variable compared with FFP. FP24 should be infused immediately after thawing or stored at 1 to 6° C. for up to 24 hours. If stored longer than 24 hours, the component must be relabeled or discarded. This plasma component serves as a source of plasma proteins for patients who are deficient in or have defective plasma proteins. Coagulation factor levels might be lower than those of FFP, especially labile coagulation Factors V and VIII.

Thawed Plasma is derived from FFP or FP24, prepared using aseptic techniques (closed system), thawed at 30 to 37° C., and maintained at 1 to 6° C. for up to 4 days after the initial 24-hour post-thaw period has elapsed. Thawed plasma contains stable coagulation factors such as Factor II and fibrinogen in concentrations similar to those of FFP, but variably reduced amounts of other factors (e.g., as show in FIG. 15).

Liquid Plasma is separated no later than 5 days after the expiration date of the Whole Blood and is stored at 1 to 6° C. The profile of plasma proteins in Liquid Plasma is poorly characterized. Levels and activation state of coagulation proteins in Liquid Plasma are dependent upon and change with time in contact with cells, as well as the conditions and duration of storage. This component serves as a source of plasma proteins. Levels and activation state of coagulation proteins are variable and change over time.

FFP and FP24 are indicated in the following conditions: management of preoperative or bleeding patients who require replacement of multiple plasma coagulation factors (e.g., liver disease, DIC); patients undergoing massive transfusion who have clinically significant coagulation deficiencies; patients taking warfarin who are bleeding or need to undergo an invasive procedure before vitamin K could reverse the warfarin effect or who need only transient reversal of warfarin effect; for transfusion or plasma exchange in patients with thrombotic thrombocytopenic purpura (TTP); management of patients with selected coagulation factor deficiencies, congenital or acquired, for which no specific coagulation concentrates are available; management of patients with rare specific plasma protein deficiencies, such as C1 inhibitor, when recombinant products are unavailable.

Thawed Plasma is indicated for: management of preoperative or bleeding patients who require replacement of multiple plasma coagulation factors except for patients with a consumptive coagulopathy; initial treatment of patients undergoing massive transfusion who have clinically significant coagulation deficiencies; and patients taking warfarin who are bleeding or need to undergo an invasive procedure before vitamin K could reverse the warfarin effect or who need only transient reversal of warfarin effect. Thawed Plasma should



not be used to treat isolated coagulation factor deficiencies where other products are available with higher concentrations of the specific factor(s).

Liquid Plasma is indicated for initial treatment of patients who are undergoing massive transfusion because of life-threatening trauma/hemorrhages and who have clinically significant coagulation deficiencies.

Various embodiments of plasma powder of the type described herein, may exhibit levels of physiological activity equivalent or superior to FFP or FP24, and thus may be suitable, e.g., for the uses of Liquid Plasma, Thawed Plasma, FP24, and FFP, as described above. For example, FIG. 15 shows the coagulation factor activity for thawed plasma derived from FFP for several coagulation factors. Plasma powder of the type described herein may exhibit substantially similar coagulation activity for one or more or all of the listed factors.

Various embodiments of plasma powder of the type described herein, may exhibit a PT (in seconds) of 48 or less, 31 or less, 15 or less, etc. For example, the plasma powder may have a PT (in seconds) in the range of 10-48, in the range of 14-31, in the range of 10-15, etc.

Various embodiments of plasma powder of the type described herein, when reconstituted, may exhibit an aPTT (in seconds) of 95 or less, 66 or less, 35 or less, etc. For example, the plasma powder may have an aPTT (in seconds) in the range of 30-95, in the range of 28-66, in the range of 30-35, etc.

Various embodiments of plasma powder of the type described herein, when reconstituted, may exhibit a Fibrinogen level (in mg/dL) of 100 or more, 110 or more, 223 or more, etc. For example, the plasma powder may have a Fibrinogen level (in mg/dL) in the range of 100-500, in the range of 110-300, in the range of 223-500, etc.

Various embodiments of plasma powder of the type described herein, when reconstituted, may exhibit a Protein C level (in IU/dL) of 54 or more, 55 or more, 74 or more, etc. For example, the plasma powder may have a Protein C level (in IU/dL) in the range of 54-154, in the range of 55-130, in the range of 74-154, etc.

Various embodiments of plasma powder of the type described herein, when reconstituted, may exhibit a Protein S level (in IU/dL) of 56 or more, 55 or more, 61 or more, etc. For example, the plasma powder may have a Protein S level (in IU/dL) in the range of 56-138, in the range of 55-110, in the range of 61-138, etc.

Various embodiments of plasma powder of the type described herein, when reconstituted, may exhibit a Factor V level (in IU/dL) of 17 or more, 30 or more, 54 or more, etc. For example, the plasma powder may have a Factor V level (in IU/dL) in the range of 17-135, in the range of 30-110, in the range of 63-135, etc.

Various embodiments of plasma powder of the type described herein, when reconstituted, may exhibit a Factor VII level (in IU/dL) of 31 or more, 30 or more, 54 or more, etc. For example, the plasma powder may have a Factor VII (in IU/dL) level in the range of 31-172, in the range of 30-110, in the range of 54-172, etc.

Various embodiments of plasma powder of the type described herein, when reconstituted, may exhibit a Factor VIII level (in IU/dL) of 10 or more, 25 or more, 47 or more, etc. For example, the plasma powder may have a Factor VIII (in IU/dL) level in the range of 10-195, in the range of 25-90, in the range of 47-195, etc.

Various embodiments of plasma powder of the type described herein, when reconstituted, may exhibit a Factor IX level (in IU/dL) of 13 or more, 25 or more, 70 or more, etc. For

example, the plasma powder may have a Factor IX level (in IU/dL) in the range of 13-141, in the range of 25-135, in the range of 70-141, etc.

Various embodiments of the plasma powder may exhibit any combination of the above activity levels.

Some embodiments of plasma powder of the type described herein may be a dry powder containing, e.g., less than 1% moisture by weight, less than 5% moisture by weight, less than 10% moisture by weight, etc. Some embodiments may have powder with moisture content in the range, e.g., of 3-5% moisture by weight.

Various embodiments of plasma powder of the type described herein, may be a fine powder having an average particle size less than 100 microns, less than 50 microns, less than 10 microns, less than 5 microns, less than 1 micron, etc. For example, the powder may have an average particle size in the range of 1-30 microns. In some embodiments, the powder has a maximum particle size of less than 100 microns, less than 50 microns, less than 10 microns, less than 5 microns, less than 1 micron, etc. For example, the powder may have a maximum particle size in the range of 1-30 microns. Such fine powders may advantageously be reconstituted quickly and efficiently, e.g., using the reconstitution techniques described herein.

Various embodiments of plasma powder of the type described herein may be composed of 10% or more, 20% or more, 30% or more, 40% or more, 50% or more dried proteins by weight. In some embodiments, when reconstituted at a ratio of 0.09 grams of powder to 1 mL of reconstituting fluid, the reconstituted plasma has a protein concentration ration of about 48 mg/mL, e.g., in the range of 45-55 mg/mL.

Advantageously, embodiments of the dried plasma powders described herein may be stored for extended storage times while maintaining a high level of physiological activity. Various embodiments of plasma powder of the type described herein may be stored in a closed sterile container (e.g., a sealed sterile bag) for a storage time, and then, upon reconstitution, exhibit any of the levels of physiological activity set forth above. For example, in various embodiments, the stored powder storage time may be up to 1 day, 1 week, 1 month, 2 months, 3 months, 4 months, 5 months, 6 months, 7 months, 8 months, 9 months, 1 year, 2 years, 5 years, or even longer. After the storage time, the powdered may be reconstituted to form a reconstituted plasma having level of physiological activity equal to or greater than, e.g., Liquid Plasma, Thawed Plasma, FP24, or FFP. Various embodiments of the dried plasma, during storage experience a rate of degradation (i.e., loss of physiological activity) comparable or less than that of e.g., Liquid Plasma, Thawed Plasma, FP24, or FFP.

FIG. 1A is a diagram of an exemplary spray drying system 100a for producing plasma powders of the type described above. The system 100a includes a spray drying apparatus 140a. A blood donor 110a donates blood 125a via a blood collection device 120a. The blood collection device 120a (e.g., needle and bag, etc.) collects blood 125a from a blood donor 110a (e.g., human). A fluid processing device 130a processes the blood 125a to separate plasma 135a from the blood 125a (e.g., a centrifuge device, a reactant, etc.).

The plasma 135a is transferred to the spray drying apparatus 140a (e.g., a pump, gravity, etc.). The spray drying apparatus 140a produces physiologically active plasma powder 145a via the spray drying techniques described herein. The physiologically active plasma powder 145a is stored in a spray dried plasma storage device 150a (e.g., a plastic bag, a glass container, a sealed bag, a sealed container, etc.).

A spray dried plasma reconstitution device 160a reconstitutes the physiologically active plasma powder 155a with a

reconstitution fluid (e.g., water, glycine, saline solution, a buffer solution, a blood substitute, etc.) to form physiologically active reconstituted plasma **165a**. In some embodiments, two reconstitution fluids can be used; e.g., in one embodiment, a mixture of distilled Water and 1.5% (200 mM glycine) (available from Baxter International Inc. of Deerfield, Ill.) is used.

The plasma powder **145a** may exhibit, a recovery rate for the protein between the plasma and the physiologically active reconstituted plasma, of at least 50%, at least 60%, at least 70%, at least 80%, at least 90%, etc. In some embodiments, the reconstituted plasma has protein levels comparable to or better than FFP or FP24. The physiologically active reconstituted plasma **165a** is administered to a plasma recipient **170a** (e.g., via an intravenous injection, applied to a wound on the plasma recipient, etc.).

In other embodiments, the blood collection device **120a** and the fluid processing device **130a** are an integrated device that collects the blood, separates the plasma from the blood, and returns the remaining parts of the blood back to the blood donor **110a**. This process can be referred to as apheresis and can, for example, utilize an apheresis device.

FIG. 1B is a diagram of an exemplary spray drying system **100b**. The system **100b** includes a spray drying apparatus **140b**. A blood collection device **120b** (e.g., needle and bag, etc.) collects blood **125b** from a blood donor **110b** (e.g., human).

A fluid processing and washing device **130b** processes the blood **125b** to separate plasma **132b** from the blood **125b** (e.g., a centrifuge device, a reactant, etc.). The fluid processing and washing device **130b** washes the plasma **132b** to remove one or more antigens (e.g., virus, allergen, etc.). The washing of the plasma **132b** by the fluid processing and washing device **130b** can reduce the antigens on the plasma **132b** by a factor of at least 100, or at least  $10^3$ , or at least  $10^4$ , or at least  $10^5$ .

The fluid processing and washing device **130b** transfers the plasma **135a** through a ultraviolet device **134b** and a fluid filter **136b** (e.g., a pump, gravity, etc.). The ultraviolet device **134b** irradiates the plasma **132b** with ultraviolet radiation to destroy one or more antigens (e.g., virus, allergen, etc.). The irradiation of the plasma **132b** by the ultraviolet radiation can reduce the antigens on the plasma **132b** by a factor of at least 100, or at least  $10^3$ , or at least  $10^4$ , or at least  $10^5$ . The fluid filter **136b** filters one or more antigens from the plasma **132b** (e.g., biofilter, activated charcoal filter, etc.). The filtering of the plasma **132b** by the fluid filter **132b** can reduce the antigens on the plasma **132b**, e.g., by a factor of at least 100, or at least  $10^3$ , or at least  $10^4$ , or at least  $10^5$ . An advantage of washing, irradiating, and/or filtering the plasma **132b** is that this process cleans the plasma **132b** so that a plurality of units of plasma can be pooled together for processing by the spray drying apparatus **140b**, thereby increasing the efficiency of the spray drying processing by allowing more plasma to be spray dried during a drying cycle. After the plasma **132b** is processed by the ultraviolet device **134b** and the fluid filter **136b**, filtered plasma **138b** is transferred to the spray drying apparatus **140b**.

The spray drying apparatus **140b** produces physiologically active plasma powder **145b** via the spray drying techniques described herein. The physiologically active plasma powder **145b** is stored in a spray dried plasma storage device **150b** (e.g., a plastic bag, a glass container, a sealed bag, a sealed container, etc.).

A spray dried plasma reconstitution device **160b** reconstitutes the physiologically active plasma powder **155b** with a reconstitution fluid (e.g., water, glycine, any suitable irriga-

tion fluid, a blood substitute, etc.) to form physiologically active reconstituted plasma **165b**. The physiologically active reconstituted plasma **165b** is administered to a plasma recipient **170b** (e.g., via an intravenous injection, applied to a wound on the plasma recipient, etc.).

In some embodiments, the reconstitution fluid includes glycine. Not wishing to be bound by theory, in some embodiments, it is believed that the glycine can enable the physiologically active reconstituted plasma **165b** to act as a volume expander and can increase the efficacy of the plasma. In some embodiments, the glycine may advantageously affect the pH level of the reconstituted plasma, thereby increasing the efficacy of the plasma. In one embodiment, the reconstitution fluid includes 1.5% glycine. In other embodiments, reconstitution fluid includes glycine concentrations of 0.1%, 0.5%, 1.0%, 1.25%, 1.3%, 1.4%, 1.6%, 1.7%, 1.75%, 2%, 2.5%, 3%, 4%, or 5%. As discussed in greater detail below, in some embodiments, plasma powder reconstituted with glycine exhibits improved PT, aPTT, and coagulation factor levels in comparison to plasma powder reconstituted with water.

In various embodiments, other reconstitution fluids may be used including, e.g., solutions including a buffering agent (e.g., a phosphate buffer, HCl, buffer Citric Acid buffer, etc.). As with glycine, these reconstitution fluids may be used to adjust the pH level of the reconstituted plasma to a desired value or range. For example, in some embodiments, the spray dried plasma may have a pH level which differs from native plasma, and a buffering agent may be used to adjust the pH level of the reconstituted plasma to more closely match that of the native plasma.

FIG. 2 is a diagram of another exemplary spray drying system **200**. The system **200** receives plasma stored in a plasma storage device **210** and includes a centrifuge device **230**, a spray drying apparatus **240**. The system **200** stores plasma powder in a plasma powder storage device **290**. The spray drying apparatus **240** includes a pump device **242**, a heated air stream device **244**, a gas supply device **246**, a spray nozzle **248**, a spray chamber **250**, a cooling/heating device **252**, a particle collection device **254**, a vacuum device **256**, and an output optimization device **258**.

The centrifuge device **230** centrifuges the plasma stored in a plasma storage device **210** to maximize the delivery of particular particles of the plasma to the spray drying apparatus **240** (e.g., platelets, protein, type of plasma, etc.). The centrifuge device **230** moves the centrifuged plasma to the spray drying apparatus **240** (e.g., directly via a pump, indirectly via gravity, etc.). Although FIG. 2 illustrates the system **200** including the centrifuge device **230**, in some embodiments of the system **200**, the centrifuge device **230** is not included in the system **200**. For example plasma obtained from any suitable source/supplier can be input into the spray drying system.

The pump device **242** pumps the plasma to the spray nozzle **248** at a set pump setting (e.g., corresponding to a flow rate of about 11.5 mL/min, in the range of 9 to 15 mL/min, etc.). In some embodiments, the plasma can be combined with the reagent or any other type of substance (e.g., blood thinner, water, glycine, blood substitute, etc.) prior to exiting the nozzle **248**. In other embodiments, the plasma is not combined with any substance.

The heated air stream device **244** provides a heated, dehumidified air stream to the spray nozzle **248** (e.g., 107° C. at 5% humidity, 109° C. at 25% humidity, etc.). Some embodiments, e.g., as described below, may include a separate heater and dehumidifier for providing the heated dehumidified stream of air.

The gas supply device **246** provides a non reactive gas (e.g., nitrogen, air, carbon dioxide, helium, etc.) at a spray flow rate (e.g., continuous, intermittent, etc.) to the spray nozzle **248**. As used herein, a non reactive gas is one which does not chemically react with the plasma or heated air stream during the operation of the spray drying system. The non reactive gas may be, e.g., an inert gas, or a non inert gas which does not react under the operating conditions of the system. In one embodiment, the spray nozzle **248** combines the non reactive gas and the plasma to atomize the plasma into the spray chamber **250**. The spray cone of atomized plasma exiting the nozzle **248** is treated by the heated air stream, to dry the atomized particles.

The cooling/heating device **252** or separate heating or cooling devices can heat and/or cool parts of the spray chamber **250** (e.g., to remove remaining moisture, to stop the denaturing of the proteins in the plasma, etc.). The particle collection device **254** collects the spray dried plasma utilizing the vacuum device **256** (e.g., via a cyclone affect). For example, the vacuum device **256** creates a vacuum that pulls the atomized particles into the particle collection device **254** (e.g., particle filter, cyclone trap, etc.). The physiologically active plasma powder is stored in a plasma powder storage device **290**. Additionally or alternatively, a pump or other similar devices may be used to provide air flow to move the particles through the collection device **254**.

The output optimization device **258** measures the output temperature of the atomized particles after they have been emitted from the spray nozzle **248**, e.g., as they enter the spray chamber **250**, at the interface between the spray chamber **250** and the collection device **254**, or at another suitable position. In some embodiments, the temperature of the particles is not measured directly; instead, an indirect indicator (e.g., an outlet gas temperature) is measured. The temperature of the atomized particles is maintained below a threshold temperature to prevent denaturing of the proteins within the plasma. The output temperature is not directly adjustable. The output optimization device **258** can adjust the pump setting of the pump device **242** and/or the input temperature of the heated air stream device **244** to maintain the output temperature in a selected temperature range.

In some embodiments, the pump setting of the pump device **242** is dynamically adjusted based on the input temperature of the plasma at the spray nozzle **248** and/or the output temperature of the spray dried plasma powder at the spray chamber **250** and/or at the particle collection device **254**.

FIG. 3A is a diagram of another exemplary spray drying system **300**. The system **300** includes a spray drying apparatus **340**. The spray drying apparatus **340** includes a peristaltic feed pump **342**, a dehumidifier/heated air supply **344**, a non reactive gas supply **346**, a nozzle **348**, a drying chamber **350**, an inlet temperature device **352**, an outlet temperature device **354**, spray dried particles **356**, a cyclone chamber **358**, a powder collection chamber **360**, a filter **362**, and a vacuum supply **364**.

The peristaltic feed pump **342** pumps plasma **310** at a pump rate (e.g., continuous, intermittent, etc.) to the nozzle **348**. The dehumidifier/heated air supply **344** heats and/or dehumidifies air, output from the vacuum supply **364** and blows a heated, dehumidified air stream at an inlet temperature to the nozzle **348**. Preferably the temperature of the air stream is adjustable. The non reactive gas supply **346** supplies a non reactive gas (e.g., nitrogen, helium, carbon dioxide, air, etc.) to the nozzle **348** at a flow rate (e.g., continuous, intermittent, etc.). In one embodiment, the non reactive gas supply **346** is a pressured tank of the non reactive gas with a regulator. In

another embodiment, the non reactive gas supply **346** is a pump for pressurizing the non reactive gas. The plasma **310**, the heated dehumidified air stream, and the non reactive gas are combined at the nozzle **348** and the atomized plasma is blown into the drying chamber **350**.

The spray dried particles **356** are moved into the cyclone chamber **358** via the vacuum created by the vacuum supply **364** for cyclonic separation. Cyclonic separation is a method of removing particulates from an air, gas or water stream, without the use of filters, through vortex separation. Rotational effects and gravity are used to separate mixtures of solids and fluids. In some embodiments, the cyclone chamber **358** is a cylindrical body with a tapered conical bottom portion. As shown in FIG. 3B, rotating (air) flow is established within the cyclone chamber **358**. Air flows in a spiral pattern, beginning at the top (wide end) of the cyclone chamber and ending at the bottom (narrow) end before exiting the cyclone in a straight stream through the center of the cyclone and out the top. Larger (denser) particles in the rotating stream have too much inertia to follow the tight curve of the stream and strike the outside wall, falling then to the bottom of the cyclone where the particles form a powder that can be collected and removed. In a conical system, as the rotating flow moves towards the narrow end of the cyclone the rotational radius of the stream is reduced, separating smaller and smaller particles. The cyclone geometry, together with flow rate, defines the cut point of the cyclone. This is the size of particle that will be removed from the stream with a 50% efficiency. Particles larger than the cut point will be removed with a greater efficiency, and smaller particles with a lower efficiency. In some embodiments, the surfaces of the cyclone chamber **358** may be treated to avoid adherence of the particles to the walls of the containers, e.g., due to electrostatic effects, by methods and compositions known in the art (e.g., silicone, Teflon, etc.).

Due to the cyclone effect within the cyclone chamber **358**, the spray dried particles **356** are collected within the powder collection chamber **360** and other particles are collected by the filter **362** (e.g., a high efficiency particulate air (HEPA) filter, a carbon filter, etc.).

In other embodiments, other particle collection devices may be used including, e.g., an electrostatic particle trap, a gravity based particle trap, a filter, etc.

The physiologically active plasma powder **390** is collected from the powder collection chamber **360** and can be, for example, stored (e.g., via storage container, etc.) and/or used (e.g., applied to a wound of a human, etc.).

In other embodiments, the powder collection chamber **360** is removable from the spray drying apparatus **340**.

In some embodiments, the processing of the plasma by the spray drying apparatus **340** is an isolated sterile system. In other words, after the spray drying apparatus **340** starts processing the plasma **310**, there is no introduction of any further liquids, solids, and/or gases into the spray drying apparatus **340** that could contaminate the plasma powder. Such a system enables the spray drying apparatus **340** to remain sterile during the processing of the plasma **310**.

In some embodiments, the spray drying apparatus **340** operates in a small batch mode. In the small batch mode, the spray drying apparatus **340** can process, e.g., one 400 mL of plasma (e.g., one unit of plasma from a single donor). In this mode of operation, the lines, drying chamber **350**, the cyclone chamber **358**, and/or the powder collection chamber **360** can be cleaned (e.g., sterilized, dipped in an alcohol bath, wiped by an alcohol wipe, etc.) between processing batches.

In some embodiments, the spray drying apparatus **340** operates in a large batch mode. In the large batch mode, the

spray drying apparatus **340** can process, e.g., hundreds of mL of plasma (e.g., multiple units of plasma from a plurality of donors). In this mode of operation, the units of plasma are pooled together for processing. An advantage to the spray drying apparatus **340** is that the units of plasma can be pooled together and then cleaned via the fluid processing and washing device **130b**, the ultraviolet device **134b**, and/or the fluid filter **135b** to provide a safe spray dried plasma powder while reducing the overhead of cleaning the spray drying apparatus **340** between batches. Alternatively, as described in greater detail below, the system may include one or more disposable portions that may be swapped out for new sterile counterparts between batches.

FIG. 4A is a diagram of an exemplary spray nozzle **440a** in a spray drying apparatus **400a**. The apparatus **400a** includes a dehumidifier/heated air supply **410a**, a heated air line **415a**, a peristaltic feed pump **420a**, a plasma line **425a**, a non reactive gas supply **430a**, and a non reactive gas line **435a**. The dehumidifier/heated air supply **410a** heats and/or dehumidifies air and pumps the heated air through the heated air line **415a** to the nozzle **440a**. The peristaltic feed pump **420a** pumps plasma through the plasma line **425a** to the nozzle **440a**. The non reactive gas supply **430a** supplies a non reactive gas through the non reactive gas line **435a** to nozzle **440a**. The non reactive gas, the plasma, and the heated air are combined at the end of the nozzle **440a** and the atomized particles **450a** exit the nozzle **440a**.

In some embodiments, the heated air line **415a** may include a sterile filter (e.g., a filter that removes microorganisms, particles, precipitates, and undissolved powders larger than 0.22 micron) located between the air supply **410a** and the spray nozzle **440a**. Similarly, a sterile filter may be positioned along the non reactive gas line **435a** and the spray nozzle **440a**. In various embodiments, the nozzle input lines **415a**, **425a**, and **435a** may include detachable connections to the air supply **410a**, the pump **420a**, the gas supply **430a**.

FIG. 4B is a diagram of an exemplary spray nozzle **440b** in a spray drying apparatus **400a**. A heated air stream **415b** from the heated air line **415a** and a plasma and non reactive gas mixture **437b** from the plasma line **425a** and the non reactive gas line **435a** is output from the spray nozzle **440b**. In this embodiment, the output of the heated air stream **415b** is via a circular output port that surrounds the output of the plasma and non reactive gas mixture **437b**. Note that, although one configuration is shown, other configurations may be used. For example, in some embodiments, the output port for the plasma and non reactive gas mixture **437b** is smaller than the output of the heated air stream **415b**.

FIG. 4C is a cross section diagram of the tip **450c** of spray nozzle **440b** showing the mixture of plasma and non reactive gas to atomize the plasma. The tip includes a first channel **452c** that delivers a flow of plasma to the end of the nozzle tip **450c**. A second channel **454c** is disposed concentrically about the first channel. The second channel **454c** delivers non reactive gas to the end of the tip, where it mixes with the flow of plasma. As described above, the atomized plasma may then be mixed with the heated air stream **415b** for drying. The mixture of plasma and non reactive gas exits a nozzle output port **456c** as an atomized plasma spray. The tip **450c** may include a central member **458c** located within and extending along the first channel **452c** to an end located in or near the nozzle output port **456c**. The end of the central member **458c** may include a feature **459c** which facilitates the atomization of the plasma. The feature **459c** (or other portions of the nozzle tip) may be made of a material which resists the build up of residue at the nozzle output port, e.g., ruby.

As illustrated in this example, the plasma and the non reactive gas are mixed together before the air stream mixes into the mixed plasma and the non reactive gas. In some embodiments, the mixture of the non reactive gas and the plasma atomizes the plasma into a spray. In some embodiments, the mixture of the heated air stream into the atomized particles of the plasma removes the moisture and dries the atomized particles to form spray dried plasma particles. Note that although in the example above, the heated air stream is directed in substantially the same direction as the atomized plasma, in some embodiments the heated air stream may be oriented in other directions (e.g., counter to the flow of the atomized plasma). In some embodiments the heated air flow may emanate from a port located at a position in the drying chamber other than on the nozzle.

FIG. 5A is a diagram of an exemplary centrifuge system **500a**. The system **500a** includes plasma **510**, a centrifuge device **530a**, and a spray drying apparatus **540**. The centrifuge device **530a** includes a centrifuge housing **532a**, a line **534**, a bladder **536**, an air supply device **538**, and a motor **539**.

The centrifuge housing **532a** rotates, via the motor **539** (e.g., direct drive system, indirect drive system, etc.), to provide inertial forces for the separation of the plasma **510** that is pumped and/or travels (e.g., gravity fed, etc.) through the line **534**. The air supply device **538** inflates and/or deflates the bladder **536** to provide for main line geometry as described herein.

Although FIG. 5A depicts the air supply device **538** included in the centrifuge housing **532a**, the air supply device **538** can be positioned at any place within or remotely located from the centrifuge housing **532a**.

FIG. 5B is a diagram of another exemplary centrifuge system **500b**. The system **500b** includes plasma A **512a**, plasma B **512b**, a centrifuge device **530b**, a spray drying apparatus A **545a**, and a spray drying apparatus B **545b**. The centrifuge device **530b** includes a centrifuge housing **532b**, a line A **535a**, a line B **535b**, a bladder A **537a**, and a bladder B **537b**.

The centrifuge housing **532b** rotates to provide centrifugal forces for the separation of the plasma A **512a** and the plasma B **512b** that is pumped and/or travels (e.g., gravity fed, etc.) through the line A **535a** and B **535b**, respectively. An air supply device (not shown) inflates and/or deflates each bladder A **537a** and B **537b** to provide for main line geometry for each of the lines A **535a** and B **535b**, respectively, as described herein.

In other embodiments, a plurality of bladders are located in parallel and in close proximate to the line A **535a**. For example, the line A **535a** is approximately located to four bladders (i.e., along the main line: Bladder A is positioned at 2 cm, Bladder B is positioned at 4 cm, Bladder C is positioned at 6 cm, and Bladder D is positioned at 8 cm) and each bladder can modify the geometry of the line A **535a** approximate to the location of the bladder.

FIG. 6A is a diagram of an exemplary bladder position A **636a** for line A **634a** in a centrifuge device **530** of FIG. 5. The geometry of the line A **634a** functions as a typical centrifugal sedimentation chamber, in which the target biological components are retained in the curve while non target components pass (i.e., Bladder Position 0).

FIG. 6B is a diagram of an exemplary bladder position B **636b** for line B **634b** in a centrifuge device **530** of FIG. 5. The geometry of the line B **634b** functions as a compression chamber, which holds and compresses the target biological component (i.e., Bladder Position +1).

FIG. 6C is a diagram of an exemplary bladder position C **636c** for line C **634c** in a centrifuge device **530** of FIG. 5. The

geometry of the line C **634c** functions to maximize target component recovery (i.e., Bladder Position 1).

FIG. 7A is a diagram of an exemplary line A **734a** for a centrifuge device **530** of FIG. 5. The line A **734a** includes a plurality of fluid lumens **735a**, **736a**, and **737a**.

FIG. 7B is a diagram of an exemplary line B **734b** for a centrifuge device **530** of FIG. 5. The line B **734b** includes a plurality of fluid lumens **735b** and **736b**.

FIG. 7C is a diagram of an exemplary line C **734c** for a centrifuge device **530** of FIG. 5. The line C **734c** includes a plurality of fluid lumens **735c** and **736c**.

FIG. 13A illustrates a spray drying system **1300**, featuring a disposable attachment **1301**. FIG. 13B is a schematic of the components of system **1300** with the attachment **1301** attached. FIG. 13C is a schematic of components of system **1300** with the attachment **1301** removed. FIG. 13D is a schematic of the attachment **1301** alone.

The system **1300** includes a plasma source **1302**, as shown, a bag of fresh or thawed frozen plasma pumped through a plasma line **1303** by a peristaltic pump **1304**. The system further includes a drying gas source **1305** including a pump **1305a** and a heater **1305b** for supplying the drying gas (e.g., heated dry air). The system also includes a non reactive spray gas source **1320**, e.g., a source of pressurized nitrogen gas.

Disposable attachment **1301** (shown in detail in FIGS. 13D-13F) includes spray nozzle assembly **1307** having a spray nozzle **1321** and a plasma input **1308** for sterile coupling to the plasma source **1302**. For example, as shown, the plasma input includes a feed tube **1303** with a sealed end for sterile connection to the plasma unit. In other embodiments, other types of sterile connectors or docks may be used.

The nozzle assembly **1307** also includes a drying gas input **1309** for connection to the drying gas source **1305**. The drying gas connection is a sterile connection, e.g., including a sterile filter. The nozzle assembly also includes a spray gas input **1319** for sterile connection to the spray gas source **1320** (e.g., as shown, a nitrogen). In some embodiments, the spray gas connection includes a sterile filter.

The attachment **1301** also includes a drying chamber **1310**, a collection device **1311**, and a storage container **1312**. As in the spray drying systems above, plasma, drying gas, and spray gas are combined at a spray nozzle of the nozzle assembly, and sprayed into drying chamber **1310**. Dried plasma powder is collected by the collection device **1311** (as shown a cyclone chamber) and transferred to the storage container **1302**. The collection device includes a gas output port **1313** which connects back to the main body of the spray drying system **1300** through a sterile filter. Gas from the output port is directed to an air conditioner **1314** which dehumidifies the gas, and circulates the dried gas back to the drying gas source **1305**. Waste fluid produced during the dehumidification is directed to a waste fluid storage container **1315**.

Attachment **1301** includes a sterile isolated spray drying environment which connects to the main body of the spray drying system only through sterile connections. Accordingly, after a spray drying run, a fresh isolated sterile spray drying environment can be obtained by simply removing the attachment **1301** and replacing it with a unused attachment. The new attachment **1301** need only be connected to the main body of the system **1300**, and nothing on the main body of the system **1301** requires sterilization. Accordingly, the system **1301** can be quickly changed over between spray drying runs, allowing for the efficient production of dried plasma powder.

One or more portions of the attachment **1301** may be collapsible for efficient storage. For example, in some embodiments, the drying chamber **1310** is collapsible, e.g., in an accordion fashion. One or more portion of attachment **1301**

may be made of a plastic or polymer material, or other suitable material (e.g., chosen for light weight, low cost, ease of fabrication, etc.).

In some embodiments, system **1300** includes a mechanism for positively identifying the attachment **1301** as an appropriate attachment for the system. The mechanism may include a bar code reader, an RFID system, etc. In one embodiment, the attachment **1310** includes a microchip that stores an encrypted code which is read by the system **1300** to verify the identity of the attachment **1301**.

In some embodiments, system **1300** includes one or more sensors, interlocks, etc., to confirm the proper attachment of the attachment **1301**. In some embodiments, the sensors are in communication with a controller which prevents operation of the system **1300** in the event of improper or incomplete attachment.

As shown, spray dry system **1300** includes a device **1316** for automatic sealing and removal of the storage container **1312**. The device **1316** may include an automated clamping and cutting mechanism, to seal of the container **1312** and remove it from the attachment **1301**.

FIGS. 14A-14D illustrate various air flow configurations for the spray dry systems of the types described herein. Referring to FIG. 14A, in one embodiment, a pump **1401** receives dry air and directs a stream of dry air to heater **1402** for heating. The heated dry air passes through sterile filter **1403**, and through a spray nozzle (not shown) into a sterile, isolated drying and particle collection chamber **1404**. The air stream is output through a second filter **1405** to an air conditioning unit **1406** for dehumidification. Dry air from the air conditioning unit **1406** is drawn in to pump **1401** to begin the cycle again. Accordingly, the air stream is recirculated in a closed loop fashion.

Referring to FIG. 14B, in another embodiment, the pump **1401** is located on the output side of drying and collection chamber **1404**. The pump **1401** draws air out of the chamber **1404** through the filter **1405**, and directs the air stream to the air conditioning unit **1406** for dehumidification. Dry air from the air conditioning unit **1406** is directed through the heater **1402** and through the filter **1403** into the drying and collection chamber **1404**. Accordingly, the air stream is recirculated in a closed loop fashion.

Referring to FIG. 14C, in another embodiment, the air stream is not recirculated in a closed loop. The pump **1401** draws in room air, and directs an air stream to the air conditioning unit **1406** for dehumidification. Dry air from the air conditioning unit **1406** is directed through the heater **1402** and through the filter **1403** into the drying and collection chamber **1404**. Air output from the chamber **1404** passes through the filter **1405** and is exhausted to an external environment.

Referring to FIG. 14D, in another embodiment, the air stream is again not recirculated in a closed loop. In this case, the pump **1401** is located on the output side of the drying and collection chamber **1404**. The pump **1401** provides negative pressure which draws room air into the air conditioning unit **1406** for dehumidification. Dry air from the air conditioning unit **1406** is directed through the heater **1402** and through the filter **1403** into the drying and collection chamber **1404**. Air is drawn out through the filter **1405** to the pump **1401**, and is exhausted to an external environment.

Note that in each of the configurations shown in FIGS. 14A-14D, the air stream passes into and out of the drying and collection chamber **1404** through sterile filters. Accordingly, the chamber is maintained as an isolated sterile environment (as indicated by the dotted box). This is the case both for the

closed loop recirculating configurations shown in FIGS. 14A-14B, and the open non circulating air stream configurations shown in FIGS. 14C-14D.

In various embodiments, spray drying systems as described herein produce waste fluid as a byproduct of the drying process. In some embodiments (e.g., in the system shown in FIG. 13A), the waste fluid is collected in a detachable receptacle, which can be discarded using the standard protocols for disposal of biomedical waste. In some embodiments, the spray drying system may be connected (e.g., hard or soft plumbed) to a treatment facility which receives and treats waste fluid from the system. In some embodiments, the spray drying system may include one or more waste treatment devices for treating the waste fluid. For example, the system may include a reservoir of treatment material (e.g., chlorine bleach), which may be mixed with the waste fluid to render it safe for disposal in a standard sewer system. In some such embodiments, the system may be connected (e.g., hard or soft plumbed) to the sewer system.

In various embodiments, the spray drying systems as described herein may include a process tracking and management capability. For example, in some embodiments, the system may include a device (e.g., bar code reader, RFID reader, etc.) that reads information. The information may include the identity, type, lot, etc. of plasma units input into the system, the identity, type, lot, etc of output dried plasma powder units, etc. This information may be processed and/or recorded using a processor (e.g., a general purpose computer) and/or a memory (e.g., a hard drive). The system may include a device (e.g., a printer) for marking input plasma or output dry plasma units with identifying information.

In various embodiments, spray drying systems as described herein may be connected, e.g., via a local area network, wide area network, the internet, etc.) to one or more external systems, databases, etc. For example the spray drying system may communicate with one or more computer systems or databases of blood centers for the purpose of process tracking and management. In some embodiments, the operation of the spray drying system may be controlled remotely. For example, in some applications, the spray drying system could be switched on or off or otherwise controlled in response to information regarding the current local need for plasma products.

FIG. 8A is a diagram of an exemplary spray dried plasma reconstitution device 860 in reconstitution system 800. The system 800 includes physiologically active plasma powder 840, the spray dried plasma reconstitution device 860, and physiologically active reconstituted plasma 890. The spray dried plasma reconstitution device 860 includes reconstitution fluid 850 and a mixer device 862 (e.g., agitation device, mixing blades, etc.).

The physiologically active plasma powder 840 and the reconstitution fluid 850 is provided to the mixer device 862. The mixer device 862 mixes (e.g., rocking, agitation, physical movement, blades, shaking, vibration, etc.) the physiologically active plasma powder 840 and the reconstitution fluid 850 (e.g., 100 mL, 200 mL, 300 mL, 400 mL, 500 mL, 600 mL, 700 mL, 800 mL, 900 mL, 1000 mL, etc.) to form the physiologically active reconstituted plasma 890. The mixer device 862 can mix the physiologically active plasma powder 840 and the reconstitution fluid 850 for a predefined (e.g., thirty seconds, two minutes, etc.) and/or a variable time period (e.g., variable time period based on an optical sensor that measures the mixing of the substances, etc.).

In some embodiments, the physiologically active plasma powder 840 and/or the reconstitution fluid 850 are connected to the spray dried plasma reconstitution device 860 via a

permanent and/or a reusable connection (e.g., syringe connection, standard medical connection, a luer taper connection, twist and lock connection, one time use connection, etc.).

In other embodiments, the mixer device 862 transfers the reconstitution fluid 850 into the bag with the physiologically active plasma powder 840. The bag with the physiologically active plasma powder 840 can be large enough to include both the physiologically active plasma powder 840 and the reconstitution fluid 850. In a further embodiment, the spray dried plasma reconstitution device can be a syringe with a nozzle (or other fluid input device) that injects the reconstitution fluid into the bag with the physiologically active plasma powder 840. In this embodiment, the bag with the physiologically active plasma powder 840 and the reconstitution fluid 850 can be rocked (manually or automatically), e.g., for thirty seconds to two minutes to mix the powder 840 and the fluid 850 together to form the physiologically active reconstituted plasma 890. As shown in FIG. 8B, a dry plasma powder storage 890 bag may be provided which includes standard input and output connectors 891 and 892 to facilitate introduction of reconstitution fluid, and output of reconstituted plasma e.g., to a standard transfusion set.

FIG. 9A is a diagram of an exemplary integrated storage and reconstitution device 900. The device 900 includes a spray dried plasma storage device 950, a spray dried plasma reconstitution device 960, a sealing mechanism 955, and a reconstitution device 957. The spray dried plasma storage device 950 includes physiologically active plasma powder 952. The dried plasma reconstitution device 960 includes reconstitution fluid 965.

The sealing mechanism 955 (e.g., plastic seal, ceramic seal, polymer seal, inter lockable connections, etc.) separates the physiologically active plasma powder 952 and the reconstitution fluid 965 from mixing before the user and/or the automated control system needs the components mixed. The user and/or the automated control system releases the sealing mechanism 955 to release the physiologically active plasma powder 952 and the reconstitution fluid 965 to the reconstitution device 957. The reconstitution device 957 reconstitutes physiologically active reconstituted plasma 990 from the physiologically active plasma powder 952 and the reconstitution fluid 965.

In some embodiments, e.g., as shown in FIG. 9B the integrated storage and reconstitution device 900 is a flexible, plastic container and the physiologically active plasma powder 952 and the reconstitution fluid 965 are each stored in a sub compartment of the plastic container. In this embodiment, the sealing mechanism 955 forms a seal between the two sub compartments. Upon release of the sealing mechanism 955, the physiologically active plasma powder 952 and the reconstitution fluid 965 mix together. In some embodiments, the reconstitution device 957 includes fins within the integrated storage and reconstitution device 900 that mix the physiologically active plasma powder 952 and the reconstitution fluid 965 together upon movement of the device 900 (e.g., shaking by the user, centrifuge by the automated control system, etc.).

FIG. 10 is a flowchart 1000 depicting an exemplary spray drying process for plasma. A user and/or an automated control system warms up (1005) the spray drying apparatus 240 of FIG. 2 (e.g., pre heats the air stream, pressurizes the apparatus via the vacuum device or pump, etc.). The user and/or the automated control system starts (1010) the spray drying

23

apparatus 240. The plasma 210 is provided (1020) to the spray drying apparatus 240. The user and/or the automated control system sets (1030) one or more parameters of the spray drying apparatus 240 (e.g., inlet temperature, outlet temperature, etc.). The user and/or the automated control system starts (1040) the spray drying process. The user and/or the automated control system collects (1050) the physiologically active plasma powder 290 from the spray drying apparatus 240.

FIG. 11 is a flowchart 1100 depicting another exemplary spray drying process for plasma. A user and/or an automated control system attaches (1110) the dehumidifier 344 to the spray drying apparatus 340 of FIG. 3. The user and/or the automated control system attaches (1115) a pre dryer to the spray drying apparatus 340, e.g., to pre heat air input to heated air supply 344 (e.g., using hot air output from a dehumidifier or other component of the system). For spray drying systems which do not use pre heating, this step may be omitted.

The user and/or the automated control system attaches (1120) glassware (e.g., the drying chamber 352, the cyclone chamber 356, the powder collection chamber 358, etc.) to the spray drying apparatus 340. Alternatively, as described in reference to FIGS. 13A-13E, a disposable attachment may be used.

The user and/or the automated control system sets (1125) the inlet temperature to a desired value on the spray drying apparatus 340. The inlet temperature can be, for example, the temperature of the air stream entering the nozzle 348. In other embodiments, the inlet temperature is the temperature of the atomized plasma as it enters the drying chamber 350. In some embodiments the inlet temperature is set to about 112° C. In various embodiments, any suitable inlet temperature may be used, e.g., an inlet temperature in the range of 85-150° C., or in the range of 100-120° C., or in the range of 110-115° C., etc.

The user and/or the automated control system sets (1130) the pump rate for the peristaltic pump 342 to a desired value. In some embodiments the pump rate is set to about 9 mL/minute. In various embodiments, any suitable pump rate may be used, e.g., a pump rate in the range of 3-14 mL/minute, or in the range of 7-11 mL/minute, or in the range of 8-10 mL/minute, etc.

The user and/or the automated control system sets (1135) the aspiration of the vacuum supply or drying gas pump to provide a flow rate out of the collection device 358 to m<sup>3</sup>/hour. In various embodiments, any suitable flow rate may be used, e.g., a flow rate in the range of 25-80 m<sup>3</sup>/hour, or in the range of 30-40 m<sup>3</sup>/hour, or in the range of 33-37 m<sup>3</sup>/hour, etc.

The user and/or the automated control system sets (1140) the flow rate from the non reactive spray gas supply 346 to a desired value, e.g., 414 L/hour. In various embodiments, any suitable flow rate may be used, e.g., a flow rate in the range of 300-500 L/hour, or in the range of 350-450 L/hour, or in the range of 375-425 L/hour, etc.

The user and/or the automated control system starts (1145) the spray drying process on the spray drying apparatus 340. The user and/or the automated control system collects (1160) the physiologically active plasma powder 390.

During the processing of the plasma 310 by the spray drying apparatus 340, an output optimization device (e.g., 261 of FIG. 2) monitors (1150) the outlet temperature of the physiologically active plasma powder 390 at the powder collection chamber 358 (or other suitable position) via the outlet temperature device 354. If the outlet temperature is substantially outside of the range of 40° C. to 44° C., the output optimization device adjusts (1155) the pump rate and/or the inlet temperature to correct the output temperature. Table 1

24

illustrates exemplary output temperatures and adjustments to the pump rate and/or the inlet temperature.

TABLE 1

Exemplary Outlet Temperatures and Respective Adjustments.				
Outlet Temperature	Set Pump Rate (mL/min)	Pump Rate Adjustment (mL/min)	Set Inlet Temperature	Inlet Temperature Adjustment
38° C.	11.5	-2	107° C.	—
39° C.	11.5	—	107° C.	+4° C.
48° C.	11.5	+1	107° C.	-1° C.
45° C.	11.5	—	107° C.	-2° C.

In general, in various embodiments, the spray drying systems described herein may feature open or closed loop control of one or more process parameters. One or more sensors (e.g., temperature sensors, flow rate sensors, pressure sensors, etc.) may be used to monitor the process. Information from these sensors (either alone or in combination) can be processed and used to control one or more process parameter (e.g., plasma flow rate, drying gas flow rate, spray gas flow rate, drying gas inlet temperature, etc.). For example, a closed servo loop may be used to control one or more sensed process parameters (e.g., drying gas outlet temperature, plasma flow rate, drying gas flow rate, spray gas flow rate, drying gas inlet temperature, etc.) at a desired value or range of values by adjusting one or more other process parameters. Process control may be implemented using any techniques known in the art, e.g., in software (e.g., run on a general purpose computer), hardware, or a combination thereof. For example, various embodiments feature closed servo loop control of the spray drying outlet temperature at a desired value (e.g., 42° C.) or range of values (e.g., 41-43° C., less than 43° C., etc.) by adjusting, e.g., the plasma pump rate, the drying gas inlet temperature, or a combination thereof. The servo loop may be implemented using any techniques known in the art, e.g., in software (e.g., run on a general purpose computer), hardware, or a combination thereof.

FIG. 12 is a flowchart 1200 depicting an exemplary process of applying physiologically active reconstituted plasma to a human patient utilizing the integrated storage and reconstitution device 900 of FIG. 9. The integrated storage and reconstitution device 900 provides (1210) the physiologically active plasma powder 952. The integrated storage and reconstitution device 900 provides (1220) the reconstitution fluid 965. The sealing mechanism 955 supplies (1230) the physiologically active plasma powder 952 and the reconstitution fluid 965 to the reconstitution device 957. The reconstitution device 957 mixes (1240) the physiologically active plasma powder 952 and the reconstitution fluid 965 to form the physiologically active reconstituted plasma 990. A user and/or an automated control system applies (1250) the physiologically active reconstituted plasma 990 to a human patient (e.g., the user, a medical user, etc.).

In some embodiments, the plasma described herein is human plasma. The plasma can be, for example, diluted (e.g., glycine, water, blood thinner, etc.) and/or undiluted (e.g., undiluted plasma separated from the blood).

In other embodiments, the parameters utilized for the spray drying apparatus are illustrated in Table 2.

25

TABLE 2

Parameters for Spray drying Apparatus			
Parameter	Setting	Range A	Range B
Inlet Temperature	107° C.	100° C. to 114° C.	102° C. to 112° C.
Pump Setting (mL/min)	11.5	7.1 to 14.4	9.5 to 12.0
Aspiration (m <sup>3</sup> /hr)	35	20 to 35	30 to 35
Spray Flow Rate (Nitrogen) (L/hr)	414	360 to 475	340 to 445
Outlet Temperature (Monitor)	NA	40° C. to 44° C.	42° C. to 43° C.

In other embodiments, the parameters utilized for the spray drying apparatus can be varied as illustrated in Table 3.

TABLE 3

Parameters for Spray drying Apparatus			
Parameter	Settings A	Settings B	Settings C
Inlet Temperature	101-113° C.	96-118° C.	85-129° C.
Pump Setting (mL/min)	9.8-12.0	9.0-13.0	18.0-15.0
Aspiration (m <sup>3</sup> /hr)	30-35	28-35	20-35
Spray Flow Rate (Nitrogen) (L/hr)	390-445	365-450	325-500
Outlet Temperature (Monitor)	38-46° C.	36-48.4° C.	32-61.6° C.

In some embodiments, (e.g., using diluted plasma) the parameters utilized for the spray drying apparatus are dependent on the protein concentration of the plasma. In other words, the parameters change based on the amount of protein per volume of the plasma. For example, in some embodiments, at 10 mg of protein per 100 ml of volume, the inlet temperature setting is 107° C. As another example, in some embodiments, at 25 mg of protein per 100 ml of volume, the inlet temperature setting is 109° C.

In some embodiments, the plasma **310** is cooled (or heated) before being pumped into the spray drying apparatus **340** by the peristaltic feed pump **342**. In this example, the bag of plasma can be cooled before being connected to the spray drying apparatus **340**.

In other embodiments, the human plasma is collected by apheresis. The human plasma can be dried and tested using the spray dry method described herein.

In some examples, the spray drying apparatus is setup per the parameters and/or steps described below. Although the following steps are numbered sequentially, the steps can occur in any order. The Buchi equipment and/or parts described herein are available from BÜCHI Labortechnik AG of Flawil, Switzerland.

1. Provide 200 ml frozen bag of plasma collected by apheresis
2. Thaw the frozen bag of plasma in a 38° C. water bath
3. Provide the Buchi B 290 spray dryer
4. Attach the Buchi B 296 dehumidifier to the spray dryer, for example, according to Buchi instructions
5. Attach Buchi pre dryer heat exchanger to the spray dryer, for example, according to Buchi instructions
6. Attach Buchi outlet HEPA filter to the spray dryer
7. Check that all glassware components are clean and dry
8. Attach Buchi high volume glassware set to the spray dryer according to Buchi instructions
9. Empty receiving bottle of Buchi B 296 dehumidifier
10. Attach thawed bag of plasma to the Buchi B 290 spray dryer
11. Set inlet temperature range of spray dryer to 107° C.

26

12. Set pump setting to 11.5 mL/minute (in other examples, the pump setting is set in a range from 7.1 to 14.4 mL/minute)

13. Set aspiration to 35 m<sup>3</sup>/hr

14. Set non reactive gas (e.g., nitrogen) flow rate to 360-475 L/hour depending on flow rate

15. Monitor outlet temperature and adjust pump rate (e.g., first adjustment) and inlet temperature (e.g., second adjustment) to keep the outlet temperature between 40-44° C.

Plasma spray drying systems of the type described herein provide for closed sterile processing of plasma into a dried plasma product. For example, referring to FIG. 16A, in some embodiments, the spray drying system **1601** receives a single unit of plasma **1602**. The plasma is processed under closed sterile conditions to produce a single unit of dried plasma in a closed sterile container **1603**. The closed sterile container **1603** may be sealed and removed for closed sterile storage. Such processing may be referred to as unit to unit processing.

Referring to FIG. 16B, in some embodiments, the spray drying system **1601** receives plasma from a pool of plasma **1604** (e.g., collected from multiple donors). The plasma is processed under closed sterile conditions to produce one or more single units of dried plasma, each in a closed sterile container **1605**. For example, plasma from the pool **1604** may be processed until a first unit of dried plasma is produced and stored in a single storage container **1605**. The storage container **1605** can then be sealed and removed from the spray dry system **1601** for closed sterile storage. A new empty sterile storage bag **1605** is attached to the spray dry **1601** system without compromising the closed environment of the system, and the process is repeated. Such processing may be referred to as pool to unit processing.

Referring to FIG. 16C, in some embodiments, the spray drying system **1601** receives multiple single units of plasma **1606** (e.g., collected from multiple donors) either in sequence or in parallel. The plasma is processed under closed sterile conditions to produce a pool of multiple units of dried plasma in a single closed sterile storage container **1607**. For example, a first unit of plasma **1606** may be attached to the spray drying system without compromising the closed sterile environment of the spray dry system **1601**. The unit **1606** is processed, and dried plasma powder collected in the storage container **1607**. Once processing of the first unit **1606** is complete, the unit **1606** and/or the storage container **1607** is removed without compromising the closed sterile environment of the spray dry system **1601**. A new unit of plasma **1606** is attached to the spray drying system **1601** while maintaining the closed sterile environment of the system, and the process repeated. Once spray dried plasma powder from several plasma units **1606** has been collected in the storage container **1607**, the storage container **1607** is sealed and removed for closed sterile storage. Such processing may be referred to as pool to unit processing.

Referring to FIG. 16D, in some embodiments, the spray drying system **1601** receives plasma from a pool of plasma **1608** (e.g., collected from multiple donors). The plasma is processed under closed sterile conditions to produce a pool of multiple units of dried plasma in a single closed sterile storage container **1609**. For example, a volume of plasma equivalent to multiple units is delivered from the pool **1608** for processed under closed sterile conditions. The resulting dried plasma powder is stored in a single storage container **1605**. After a desired amount of powder is collected, the storage container **1609** can then be sealed and removed from the spray dry system **1601** for closed sterile storage. Such processing may be referred to as pool to pool processing.



In various embodiments, a single spray drying system may operate in multiple modes corresponding to some or all of the above described processing schemes (unit to unit, pool to unit, unit to pool, pool to pool, etc.). Advantageously, such systems may switch between modes without requiring substantial reconfiguration of the system.

Example I

Table 4 illustrates test results between fresh frozen plasma, spray dried plasma rehydrated with 2 mL of water, and spray dried plasma powder rehydrated with 2 mL of glycine. The text results were obtained using a STart® 4 semi automated homostasis analyzer available from Diagnostica Stago, Inc. of Parsippany, N.J. Note that the Factor V and Factor VII values of the FFP are presented as a clotting time value with units of seconds, and not as an absolute level in units of IU/dL.

TABLE 4

Spray dried Plasma vs. Fresh Frozen Plasma					
	Total Protein (mg/mL)	Percentage of Protein Compared to Fresh Frozen Plasma	Prothrombin Time (PT) (sec)	Factor V (sec)	Factor VII (sec)
Fresh Frozen Plasma					
	50	NA	15	15	16
Spray Dried Plasma rehydrated with 2 mL water					
100 mg	31	61%	18	18	16
200 mg	56	111%	16	16	16
300 mg	78	155%	19	20	19
Spray Dried Plasma rehydrated with 2 mL glycine					
100 mg	35	69%	18	16	16
200 mg	61	121%	15	15	16
300 mg	82	163%	16	16	16
400 mg	97	193%	18	17	17

Example II

FIG. 17A shows a chart which illustrates the results of tests on spray dried plasma samples. Fresh plasma (<24 hour from draw) was dried under varying processing conditions. A first set of dried plasma units was dried with an inlet temperature of 97° C. and a fixed plasma flow rate of 3 mL/min. A second set was dried with a drying gas inlet temperature of 97° C. and with a plasma flow rate which was varied to maintain a desired gas outlet temperature. A third set was dried with a drying gas inlet temperature of 112° C. and with a plasma flow rate which was varied to maintain a desired gas outlet temperature. A fourth set was dried with a drying gas inlet temperature of 117° C. and with a plasma flow rate which was varied to maintain a desired gas outlet temperature.

A sample from each of the dried units was reconstituted in deionized water (e.g., at a ratio of 0.09 g of powder per mL of deionized water). The reconstituted plasma was tested with a Stago Compact series analyzer available from Diagnostica Stago, Inc. of Parsippany, N.J. The samples were tested for PT, aPTT, Fibrinogen Level, levels of Factors V, VII, VIII, and IX, Protein C level, and Protein S level. The results are presented in FIG. 17A.

FIG. 17B shows a chart which illustrates the results of tests on spray dried plasma samples. Fresh plasma (<24 hour from draw) was dried under varying processing conditions. The samples were run at various inlet temperatures ranging from

97-112° C. (batches labeled 2010-102 and 2010-104 at 97° C.; batches labeled 2010-040 through 2010-074 at 112° C., and batches labeled 2010-081 and 2010-083 at 117° C.). In each case, the plasma flow was varied to maintain a desired gas outlet temperature.

Each sample was reconstituted using a glycine solution (e.g., at a ratio of 0.09 g of powder per mL of reconstitution fluid). The reconstituted plasma was tested with a Stago STA series analyzer available from Diagnostica Stago, Inc. of Parsippany, N.J. The samples were tested for PT, aPTT, Fibrinogen Level, levels of Factors V, VII, VIII, and IX, Protein C level, and Protein S level. The results are presented in FIG. 17B.

DEFINITIONS

aPTT—Activated Partial Thromboplastin Time is a performance indicator known in the art measuring the efficacy of both the “intrinsic” (sometimes referred to as the contact activation pathway) and the common coagulation pathways.

PT—Prothrombin Time is a performance indicator known in the art of the extrinsic pathway of coagulation.

FGN—Fibrinogen (also referred to in the art as Factor I) is an asoluble plasma glycoprotein, synthesized by the liver, that is converted by thrombin into fibrin during coagulation.

PC—Protein C is also known as autoprothrombin IIA and blood coagulation Factor XIV, is an inactive protein, the activated form of which plays an important role in managing blood clotting, inflammation, cell death and the permeability of blood vessel walls in humans and other animals.

PS—Protein S is a vitamin K-dependent plasma glycoprotein synthesized in the endothelium. In the circulation, Protein S exists in two forms: a free form and a complex form bound to complement protein C4b. In humans, protein S is encoded by the PROS1 gene. The best characterized function of Protein S is its role in the anti coagulation pathway, where it functions as a cofactor to Protein C in the inactivation of Factors Va and VIIIa. Only the free form has cofactor activity.

Factors—As used here a “Factor” followed by a Roman Numeral refers to a series of plasma proteins which are related through a complex cascade of enzyme-catalyzed reactions involving the sequential cleavage of large protein molecules to produce peptides, each of which converts an inactive zymogen precursor into an active enzyme leading to the formation of a fibrin clot. They include: Factor I (fibrinogen), Factor II (prothrombin), Factor III (tissue thromboplastin), Factor IV (calcium), Factor V (proaccelerin), Factor VI (no longer considered active in hemostasis), Factor VII (proconvertin), Factor VIII (antihemophilic factor), Factor IX (plasma thromboplastin component; Christmas factor), Factor X (Stuart factor), Factor XI (plasma thromboplastin antecedent), Factor XII (hageman factor), and Factor XIII (fibrin stabilizing factor).

Although the methods and apparatuses described herein are described as processing/utilizing plasma, the method and apparatuses described herein can, for example, be utilized to process/utilize any type of blood product (e.g., whole blood, blood platelets, red blood cells, blood serum, etc.).

Comprise, include, and/or plural forms of each are open ended and include the listed parts and can include additional parts that are not listed. And/or is open ended and includes one or more of the listed parts and combinations of the listed parts.

One or more documents are incorporated by reference in the current application. In the event that the meaning of a

technical term in an incorporated document conflicts with the current application, the meaning in the current application is controlling.

One skilled in the art will realize the invention may be embodied in other specific forms without departing from the spirit or essential characteristics thereof. The foregoing embodiments are therefore to be considered in all respects illustrative rather than limiting of the invention described herein. Scope of the invention is thus indicated by the appended claims, rather than by the foregoing description, and all changes that come within the meaning and range of equivalency of the claims are therefore intended to be embraced therein.

What is claimed is:

1. An attachment for a plasma spray drying apparatus comprising:

a plasma inlet port for providing sterile communication to a plasma source;

a spray gas inlet port for providing removable sterile communication to a pressurized gas source;

at least one drying gas inlet port for providing removable sterile communication to a drying gas source;

a spray dry nozzle in fluid communication with the plasma and spray gas inlets;

a drying chamber in fluid communication with the attached spray nozzle and drying gas inlet to receive a spray of plasma for drying;

a particle collection device configured to collect spray dried plasma from an outlet of the drying chamber; and a collection device gas outlet port in sterile fluid communication with the collection device;

wherein the spray nozzle, drying chamber, and collection device define a sterile isolated interior volume;

wherein the at least one drying gas inlet port is non-coaxial with at least one of the plasma inlet port, the spray gas inlet port, the spray dry nozzle, or any combination thereof.

2. The attachment of claim 1, wherein the attachment comprises a sterile isolated spray drying environment.

3. The attachment of claim 1, wherein at least one of the inlet and outlet ports comprises a sterile filter.

4. The attachment of claim 1, wherein at least one of the drying chamber and the particle collection device is at least partially collapsible.

5. The attachment of claim 1, wherein the attachment is at least partially collapsible.

6. The attachment of claim 1, wherein at least part of the attachment is at least partially collapsible in an accordion fashion.

7. The attachment of claim 1, further comprising a mechanism for positively identifying the attachment.

8. The attachment of claim 7, wherein the mechanism for positively identifying the attachment comprises a bar code, a microchip, a radio frequency identification device (RFID), or any combination thereof.

9. The attachment of claim 1, further comprising one or more sensors to confirm proper attachment to the plasma source, the pressurized gas source, the drying gas source, or any combination thereof.

10. The attachment of claim 1, further comprising one or more sensors to monitor the attachment.

11. The attachment of claim 10, wherein the one or more sensors comprise a temperature sensor, a flow rate sensor, a pressure sensor, or any combination thereof.

12. The attachment of claim 1, wherein the particle collection device comprises a closable sterile storage container to store spray dried plasma.

13. The attachment of claim 12, wherein the closable sterile storage container is sealable by a device for automatic sealing of the particle collection device.

14. The attachment of claim 12, wherein the closable sterile storage container sealable by a device for automatic sealing and removal of the particle collection device.

15. The attachment of claim 1, wherein the attachment comprises a plastic or polymer material.

16. The attachment of claim 1, wherein the particle collection device comprises a cyclone chamber.

17. The attachment of claim 1, wherein the drying chamber comprises a cyclone chamber.

18. The attachment of claim 1, wherein the particle collection device comprises a sterile detachable storage portion configured to receive collected spray dried plasma.

19. The attachment of claim 1, wherein the attachment is disposable.

20. The attachment of claim 1, wherein the plasma inlet port comprises a feed tube with a sealed end for sterile attachment to the plasma source.

21. An attachment for a plasma spray drying apparatus comprising:

a spray nozzle assembly comprising:

a plasma input for sterile communication to a plasma source,

a drying gas input for sterile communication to a drying gas source,

a spray gas input for sterile communication to a spray gas source, and

a spray nozzle for combining plasma from the plasma input, a drying gas from the drying gas input, and spray gas from the spray gas input and spraying the combination of the plasma, drying gas, and the spray gas into a drying chamber; the drying chamber to dry the sprayed combination of the plasma, drying gas, and the spray gas;

a collection device to collect dried plasma powder; and a storage container to store the collected dried plasma powder;

wherein the at the drying gas input is non-coaxial with at least one of the plasma input, the spray gas input, the spray dry nozzle, or any combination thereof.

22. The attachment of claim 21, wherein the attachment comprises a sterile isolated spray drying environment.

23. The attachment of claim 21, wherein the collection device comprises a gas output port to collect gas from the attachment, the gas output port comprises a sterile filter.

\* \* \* \* \*